



USER GUIDE

Raypicker Vision software
Borea Connect

Version 1.0 - 01.2022
Ref. UG.RPV.BC.EN.1.0

RAYPLICKER VISION & BOREA CONNECT USER GUIDE

Document version 1.0

Ref. UG.RPV.BC.EN.1.0 / date 01.2022

Compatible with the Rayplicker Vision software version 1.0.1

© Copyright, BOREA SAS.

This document is the property of BOREA SAS and can not be used, reproduced or communicated to third parties without its written authorization.

The most recent version is always available on:
www.borea-dental.com

TABLE OF CONTENTS

1.	ABOUT THIS USER GUIDE	5
1.1.	Dear customers	5
1.2.	Licenses, trademarks and other rights	6
1.3.	Software purpose and users	6
1.4.	Disclaimer	7
2.	RAYPLICKER VISION REGISTRATION AND PREVIEW	8
2.1.	System requirements (PC / Mac)	8
2.2.	Installing the Rayplicker Vision	8
2.2.1.	Software Download	8
2.2.2.	Account creation	10
2.3.	Settings	12
2.3.1.	User account	12
2.3.2.	Software and device parameter	12
2.4.	Notifications and Tutorials	14
2.4.1.	Notifications	14
2.4.2.	Tutorials	14
2.5.	Software Illustrations	14
3.	THE WORKFLOW WITH RAYPLICKER VISION 15	
3.1.	Workflow by patients	16
3.1.1.	List of Patients (Dentiste account)	16
3.1.1.1.	Create a patient	16
3.1.1.2.	Find a patient	18
3.1.1.3.	Modify/delete a patient file	18
3.1.2.	Patient interface (Dentist account)	19
3.1.2.1.	Add a file to the Patient Interface	21
3.1.2.1.1.	Add a shade	21
3.1.2.1.3.	Import a patient picture	23
3.1.2.2.	Selection via dental chart	25
3.1.2.3.	Items & Order Tabs	25
3.1.3.	Shade viewer	28
3.1.4.	Create an order (Dentist account)	32
3.2.	The workflow per data	34
3.2.1.	Add a data (Dentist account)	34
3.2.1	Filter / Consult data	34
3.2.3.	Manage data	35

4.	REGISTRATION & OVERVIEW OF BOREA CONNECT	36
4.1.	Account creation	36
4.2.	Dashboard	37
4.3.	The Rayplicker community	38
4.4.	Account settings	39
5.	BOREA CONNECT - SEND AN ORDER	39
5.1.	Finalize the order on Borea Connect	39
5.2.	Send the order to the laboratory	42
6.	RECEIVE THE ORDER AT THE LABORATORY	43
6.1.	Receive the order via Borea Connect	43
6.1.1	Interpret the order	43
6.1.2.	Change order status / finalize order	45
6.2.	Receive the order on the Rayplicker Vision	46
6.2.1.	Order tab	46
6.2.2.	Manage customers	47
7.	ANNEX	48
7.1	Port configuration	48
7.2	Regulatory	48
7.3	General Data Protection Regulation	49
7.4	Contact	49

1. ABOUT THIS USER GUIDE

1.1. Dear customers

You are now equipped with the Rayplicker Vision software, congratulations on that.

This collaborative tool was created to simplify communication between dental surgeons and dental laboratories, with the common and constant objective of patient satisfaction.

Rayplicker Vision handles multiple digital workflows, including the shade taking process using the Rayplicker Handy spectrophotometer; sending and receiving the order (via the Borea Connect); as well as other processes through useful and varied features.

Precise and ergonomic, the Rayplicker solution also comes with the "Pics App Solution" application which will allow you to add patient photos to your order form, which are essential for the proper production of a prosthesis.

In order to make the best use of your shade analyzer and to optimize your digital workflow, please read this user manual carefully.

Forget approximate measurements and gain in efficiency and performance with the Rayplicker solution.

Borea team.



1.2. Licenses, trademarks and other rights

Your software is protected by a license agreement and may be used only in accordance with the terms of that agreement. Copying or using this software in any other way, except as permitted by the license agreement, is illegal.

Some of the products and accessories mentioned in this manual may not be available in all countries. Contact the manufacturer for additional information.

Trade names and trademarks:

Borea, Rayplicker Vision, Rayplicker Handy, and Borea Connect are registered trademarks of Borea. All other brands and logos mentioned in this document are trademarks, registered trademarks or logos of their respective owners.

Copyright:

The partial or complete reproduction or distribution of Borea documents is authorized only with the written consent of Borea.

Data protection:

In order to protect the data of users of the Rayplicker Vision software, Borea has implemented several security mechanisms:

- Data encryption during storage and transfer via Internet/Cloud.
- Archiving/export system to save patient data.
- Anonymization function on request to ensure the protection of patient privacy.

1.3. Software purpose and users

Software purpose:

Rayplicker Vision is free access software allowing the recovery, analysis and transmission of shade acquisitions obtained with a Rayplicker Handy device.

Indication:

This software and its Borea connect platform are used to analyze and transmit the colorimetric and translucency characteristics of a referent tooth in order to produce a dental prosthesis that will integrate itself naturally into the patient's mouth.

Benefit:

By respecting the user protocol indicated in this manual, this software makes it possible to obtain a prosthesis that conforms aesthetically (shade and translucency) to the reference tooth analyzed for natural integration in the mouth and meets the aesthetic requirements of the patient.

Patients:

This software is intended for prosthetic and aesthetic treatments on the following patients:

- Patient of all age.
- Patient requiring a prosthesis for dental care related to:
 - o the loss and/or extraction of a tooth. A single missing tooth can cause several dental problems: gum or aesthetic problems, migration or premature wear of other teeth, digestive disorders due to insufficient chewing, etc.
 - o very damaged teeth: in particular when the tooth or teeth are too damaged or dilapidated due to dental caries, or when the tooth had to be devitalised.

Users:

The Rayplicker vision software and the Borea Connect are used only by the dental surgeon or by the dental technicians.

No training is required to use the Rayplicker vision software.

The installation as well as the proper use of the Rayplicker is the responsibility of the user. For this, Borea provides the necessary information on the basis of the quick start as well as the user guide.

1.4. Disclaimer

Rayplicker Vision software is designed to be used by people with appropriate and necessary knowledge in the field of dentistry and dental technology.

The user of Rayplicker Vision software is solely responsible for the accuracy, completeness and adequacy of all data entered into this software.

Rayplicker products should be used in accordance with the accompanying instructions. Improper use or handling of Rayplicker products will void their warranty provided, if any. If you need additional information on the proper use of Rayplicker products, we invite you to contact your local distributor, or the manufacturer. The user is not authorized to modify Rayplicker products.

In the event of non-compliance with good usage practices, the residual risks impacting or likely to impact the patient are:

- Placement of a crown with a non-conform shade.
- Increased time needed to order the prosthesis.



Please backup your data at regular intervals. It is the user's responsibility to make and maintain backups to prevent data loss due to system crash or hardware failure.

At the same time, Borea recommend:

- To export data or an order from Rayplicker Vision 30 days after its creation / import, before automatic definitive deletion.
- To export an order from Borea Connect 30 days after it has been sent / received, before automatic definitive deletion.

2. RAYPLICKER VISION REGISTRATION AND PREVIEW

2.1. System requirements (PC / Mac)



Configuration	Minimum	Recommended
Windows® operating system	Windows 8 64 bits	Windows 10
Processor :	Intel Core i7	Intel Core i7
RAM :	4 Go	8 Go
Hard disk:	SSD 500 Go	SSD 500 Go
USB port :	USB 2.0 x 1	USB 2.0 x 1
Screen resolution:	1080 p	1080 p
Internet:	High speed connection	High speed connection

Using Rayplicker Vision software on a computer with insufficient minimum system requirements may result in the inability to use the software

The Rayplicker vision software is currently only available for Windows. If your operating system is lower than windows 8, the installation of the Rayplicker vision software is not possible. The same is true for Mac computer users.

An old version of the Rayplicker software is however available for download on the Borea website.

This older version, «Rayplicker software 1.201» works with the Rayplicker Handy as well as the mobile application «Rayplicker Pics App solution». It is however incompatible with the Borea connect but it integrates its own communication platform.


For more information, please contact your distributor or Borea.

Optional software: Supremo, TeamViewer, Anydesk, allowing remote technical assistance, as well as a PDF file reader to read order form or archives.

2.2. Installing the Rayplicker Vision


2.2.1. Software Download

After verifying that the system requirements is compatible with your hardware, download the Vision software from <https://borea-dental.com/products/rayplicker-vision/>

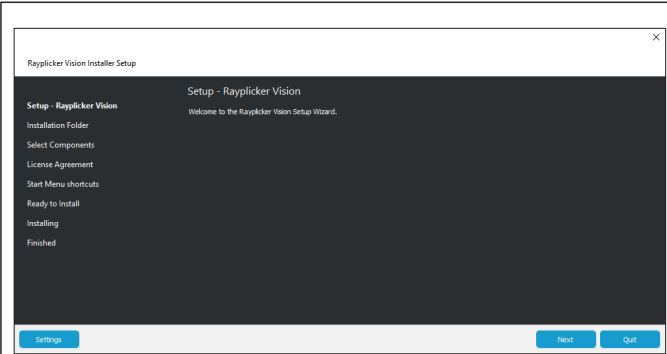

Double-click on the "Rayplicker_vision_installer" file to begin installing the software.

Click on next.

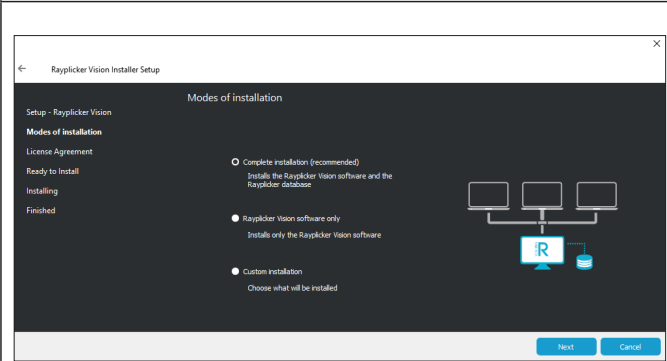


Select the desired installation mode.


- Complete installation.
- Installation of the Rayplicker software alone
- Custom installation.

Follow the instructions on the various screens.


Click on «Finish» to complete the installation.

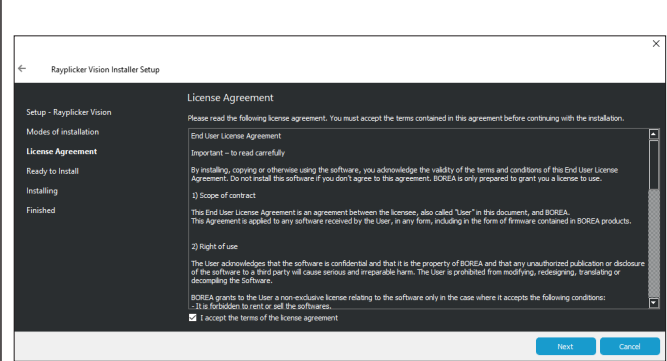





Read and accept the terms of the license agreement and click on next.

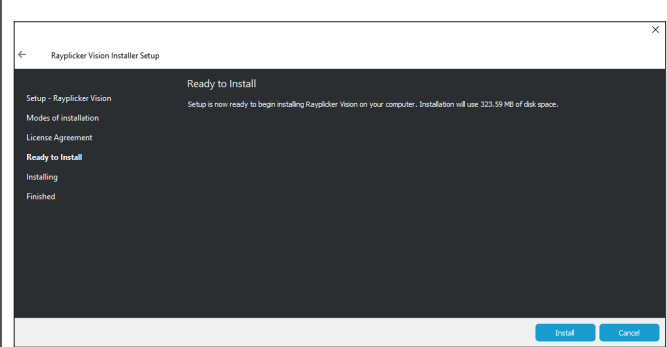


Ready for installation: click on "install".

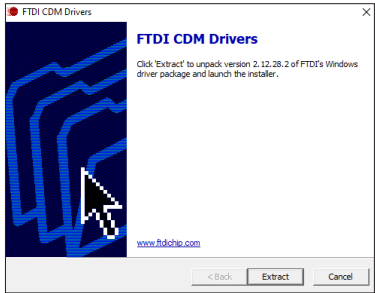

Extract the FTDI CDM drivers.

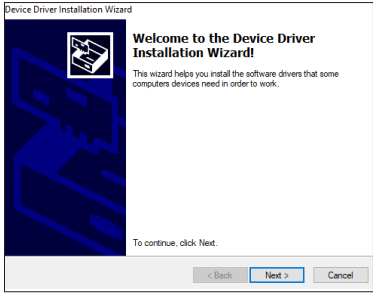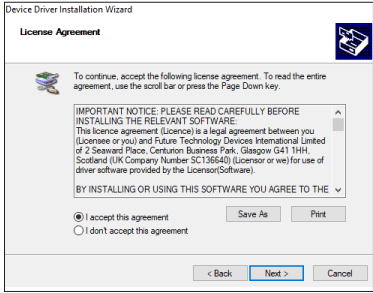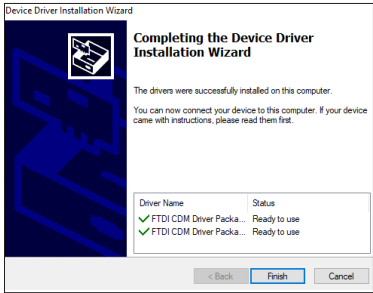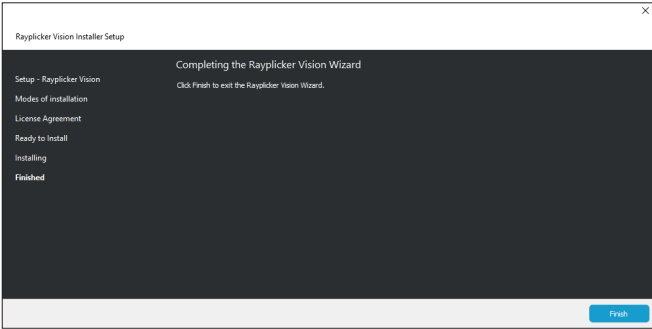	<p>Click on “next”.</p>
	<p>Accept the conditions and click on “next”.</p>
	<p>Click on «finish» to finalize the installation of the drivers.</p>
	<p>Click on “finish” to finalize the installation of the Rayplicker Vision software.</p>


2.2.2. Account creation

	<p>Click on the server of your choice.</p> <p>In the case of a standard installation, only one choice is available.</p>
---	---




First choose between a Dentist account (Allows to send files to a laboratory) and a Laboratory account (Allows to receive files from a practice).

Follow the steps of the on-screen interactive tutorial in orange.

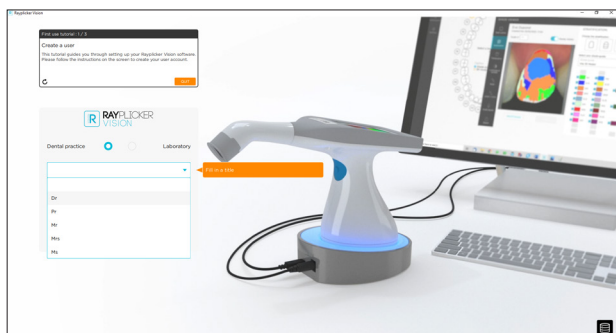

Enter the requested information (possible title, first name, last name)

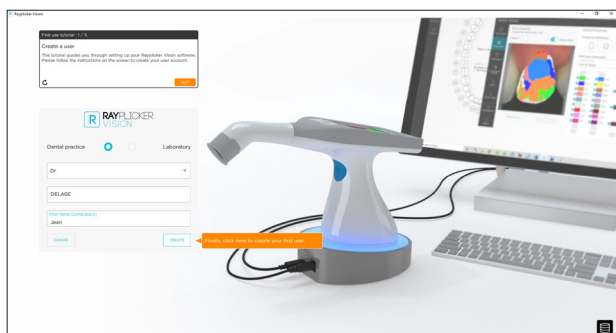

Click on create to finalize the creation of the user profile.




Once this information has been completed, a welcome window is displayed.


Click on a user to open the work session.

Click on "Add user" to create a new user.

2.3. Settings


2.3.1. User account


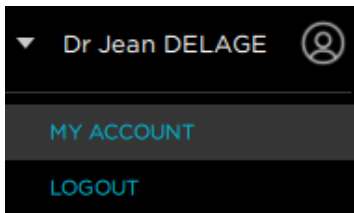
	<p>Finish setting up the account by clicking on the user name at the top right, then “My account”.</p>
---	--

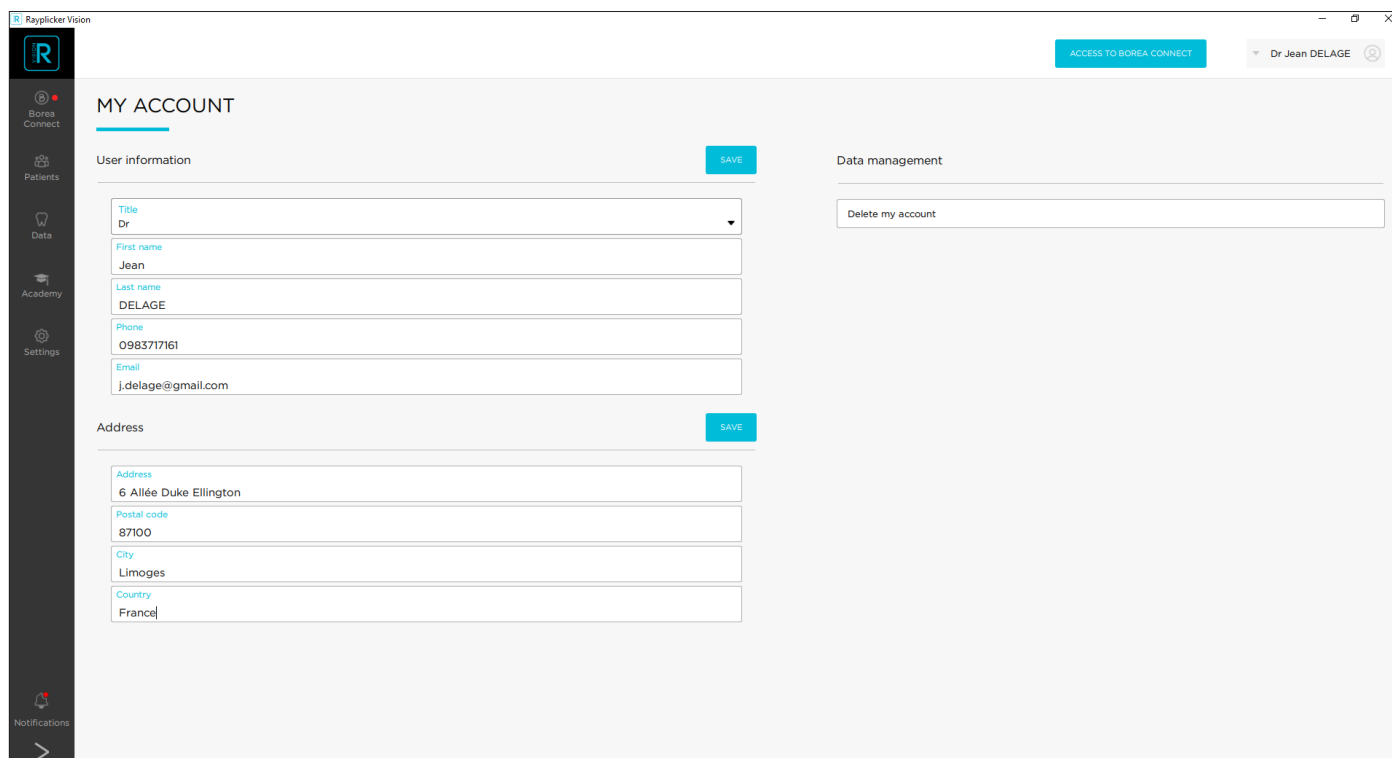

Here is personal information such as the dental practice email address or postal address. This information will be indicated on the pdf reports generated from the Rayplicker Vision software. From this interface, it is also possible to delete the account and data.

2.3.2. Software and device parameter


	<p>Other parameters are accessible via the toolbar on the left of the screen, by clicking on the «Settings» icon.</p>
---	---

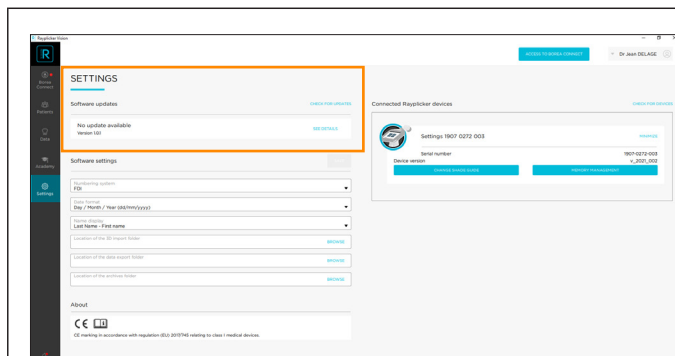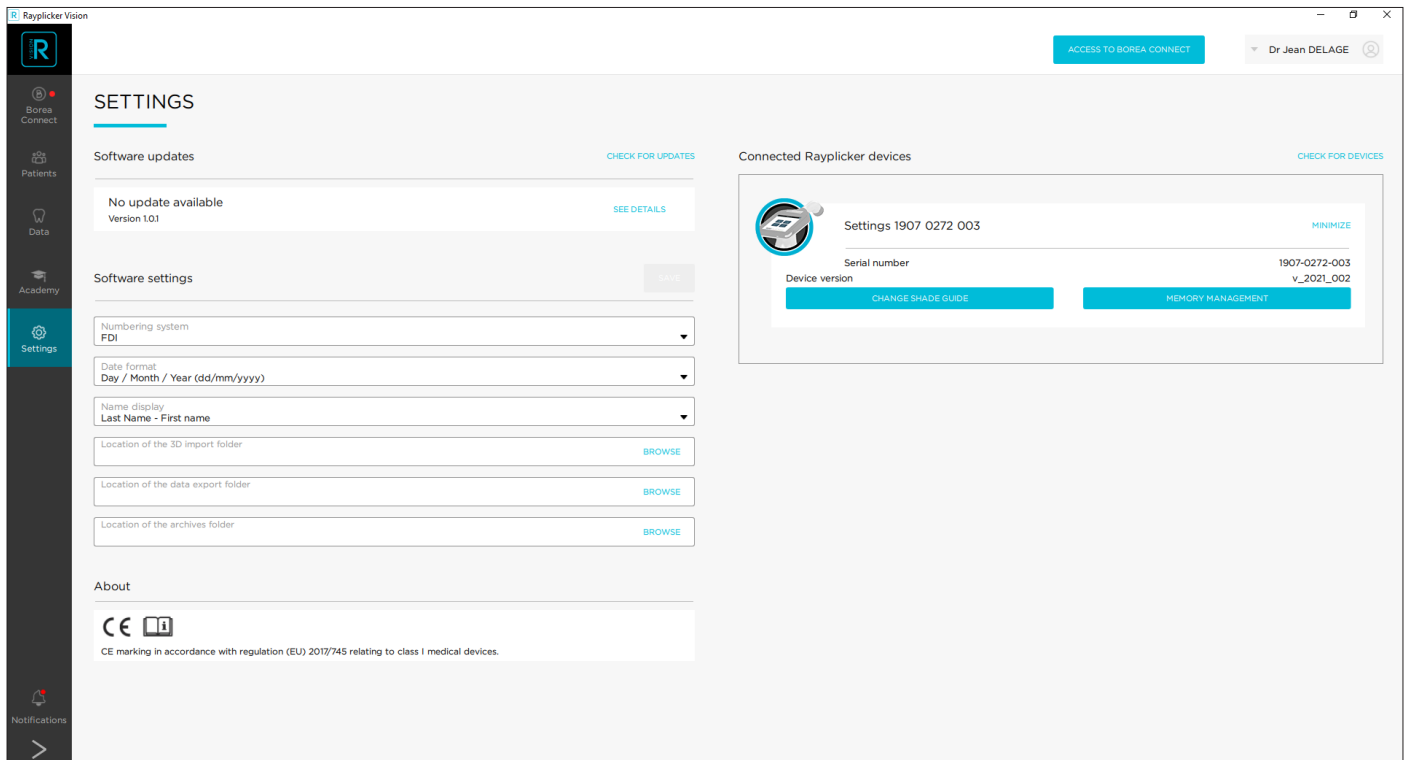

If a Vision software update is available, it is listed under Software Update.


Click on [CHECK FOR UPDATES](#) to show pending updates.

Click on [SEE DETAILS](#) to know the content, and on «Update» to download it.

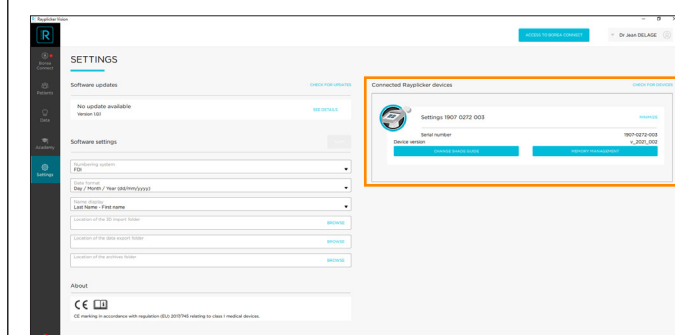

In the upper right part are indicated the connected devices.

From this interface, configuration of the connected unit reference shade guide and unit memory management is available.

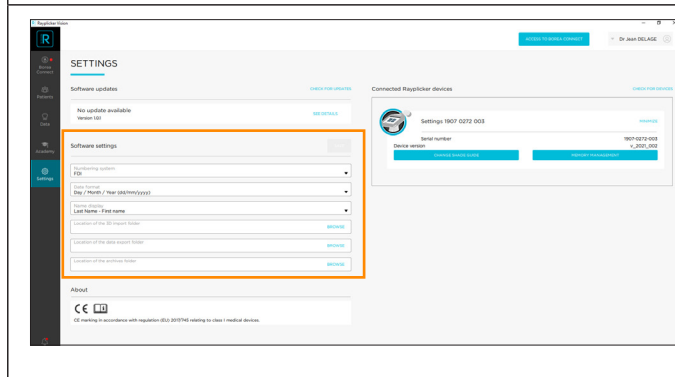


«Software settings» allows modification of the software parameters:



- The unit of measurement (metric or imperial)
- The date format.
- The tooth numbering system
- The import and export files target folders.

2.4. Notifications and Tutorials

2.4.1. Notifications





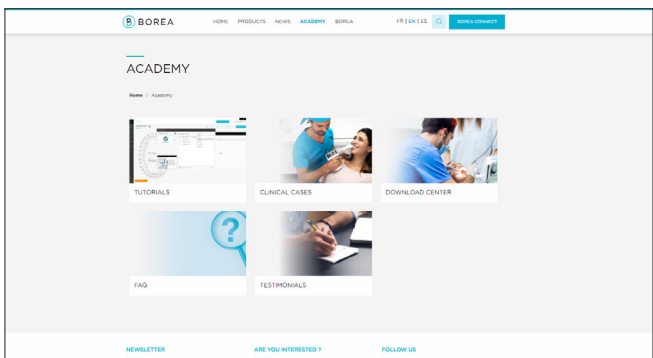

















	<p>Still via the toolbar on the left of the screen is access to notifications.</p> <p>They announce events like</p> <ul style="list-style-type: none"> - An update available for the Rayplicker Vision, - An update available for the embedded software of your Rayplicker Handy device, - The publication of a webinar or a clinical case sponsored by Borea, - The provision of supporting documents, - The presence of Borea at a trade show, congress, conference, etc.
---	--

2.4.2. Tutorials

 	<p>Still via the toolbar on the left of the screen is access to the Academy.</p> <p>From this tab, the user accesses the Academy page of the Borea website. There are available tutorials on the use of Rayplicker Vision, clinical cases, various support documents for download under the «Download center» tab, FAQs and user testimonials.</p>
---	--



2.5. Software Illustrations

Some illustrations are not directly described in the Vision software. Here is their meaning.


					
Information	Delete	Refresh	Picture file	3D file	Rayplicker file
					
Overall shade	3 parts shade	9 parts shade	Detailed mapping	Shade guide selection	Lock the area
					
Unlock the area	Zoom in	Zoom out	Type of comparison area	Invert	Tooth number is missing
					
Selected shade	Unselected shade	No viewer available	PDF file		

3. THE WORKFLOW WITH RAYPLICKER VISION

The Raypicker Vision software allows dental practitioners to work according to two different workflows. By patient or by type of data.

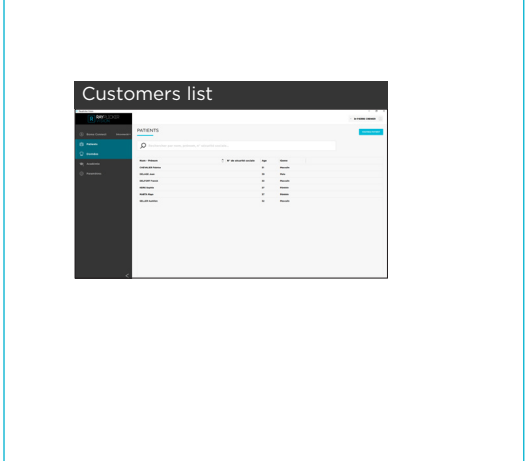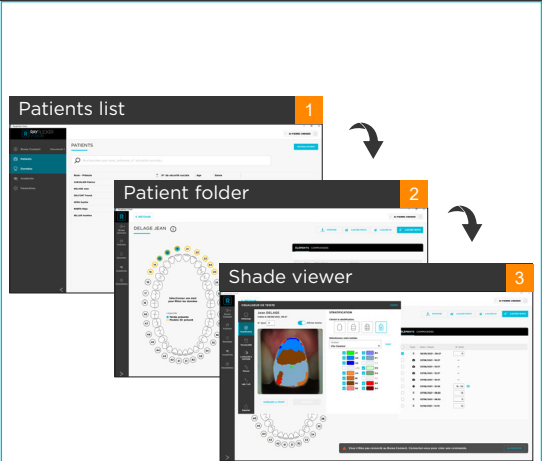


OR

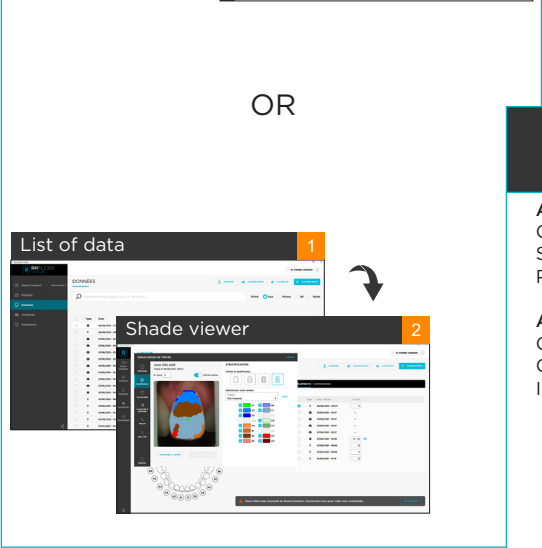

At the dental practice:
Creation of the order form
Sending the order
Progress monitoring


At the lab:
Consultation of orders
Order download
Information on the state of progress

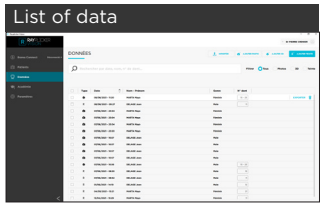


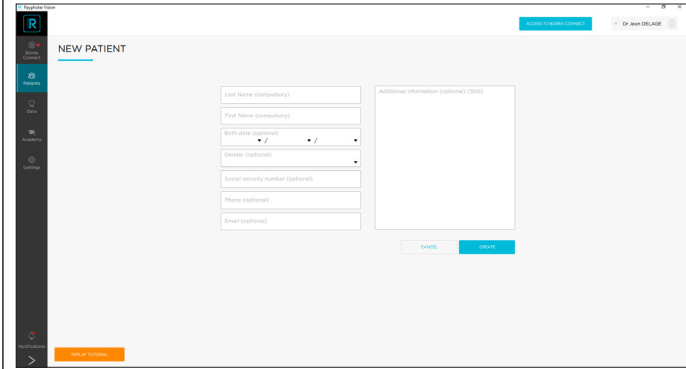
3.1. Workflow by patients

3.1.1. List of Patients (Dentiste account)

The Patients interface displays a list of all patients, their social security number, age, and gender.

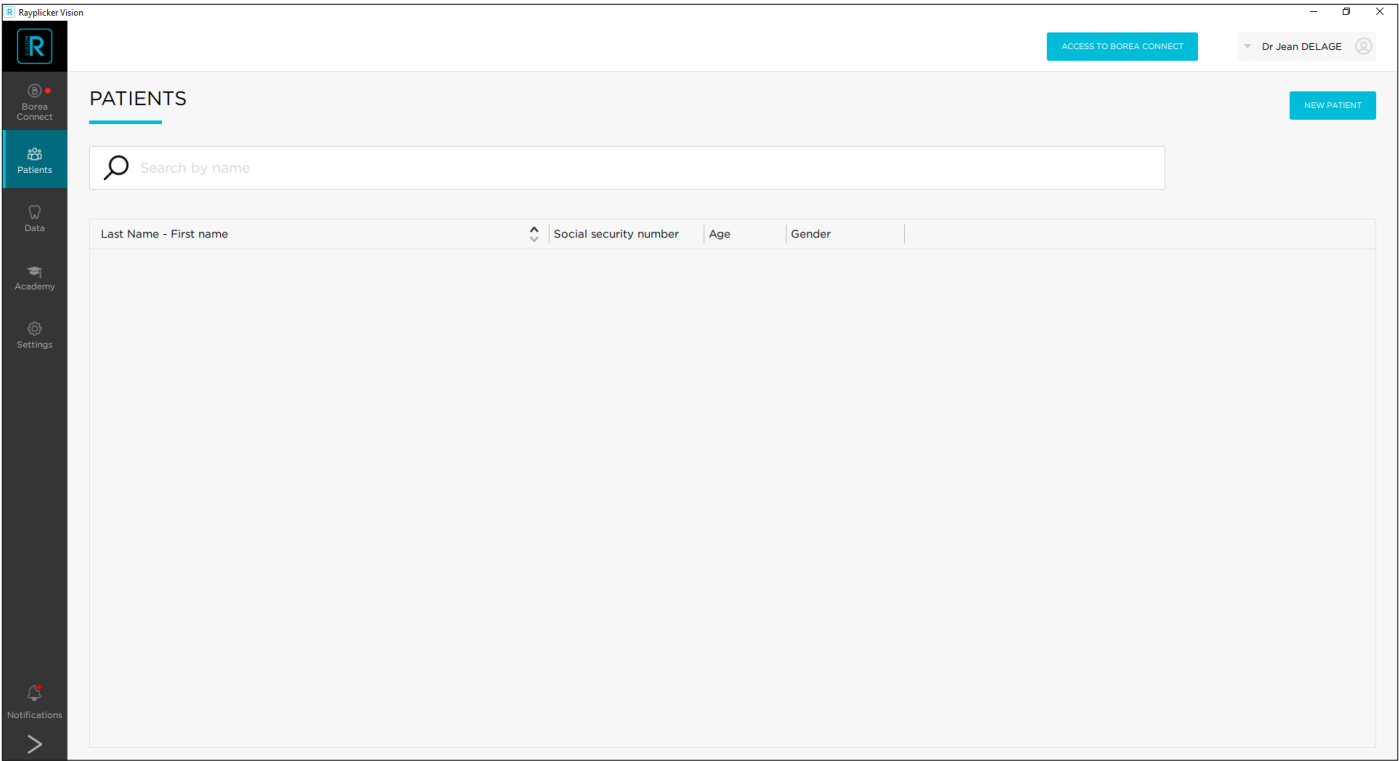

3.1.1.1. Create a patient

	<p>Click on NEW PATIENT (top right) to create a new patient file.</p>
	<p>His identification sheet opens in a new window.</p> <p>Enter at least the first and last name. Other optional information can be added:</p> <ul style="list-style-type: none">- Date of Birth- Social Security number- Phone- E-mail <p>A free field is available on the right side.</p>

CREATE

Click on CREATE to validate the entry.

Patients are added to your list (as below). Various options are then available to you.

Raypicker Vision

R

Borea Connect

Patients

Data

Academy

Settings

Notifications

ACCESS TO BOREA CONNECT

Dr. Jean DELAGE




NEW PATIENT

PATIENTS



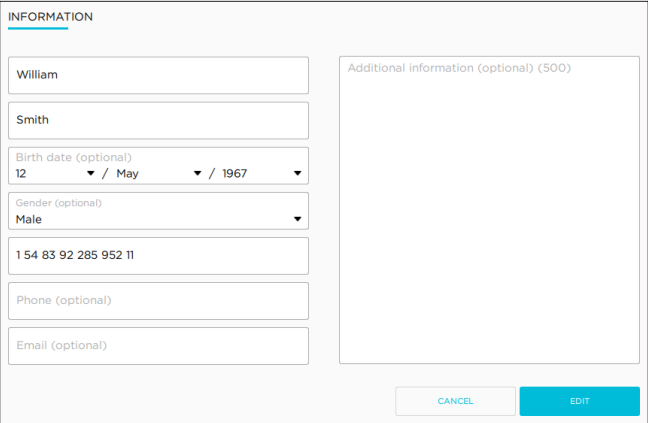


Search by name

Last Name - First name	Social security number	Age	Gender
DUPOND Eva	1 89 92 92 888 778 23	37	Female
HELEN Brook	8 23 78 87 241 854 09	36	Male
LISE Dupuis	1 59 92 22 708 208 29	42	Female
MARC Dufour	6 65 82 56 832 458 67	24	Male
REMI Durand	1 76 92 95 887 778 29	48	Male
SOPHIE Hugo	4 76 43 54 666 728 12	49	Female
WILLIAM Smith	1 54 83 92 285 952 11	54	Male


3.1.1.2. Find a patient

	<p>Click on the search text field. Enter the patient's name or social security number.</p>
	<p>Click on the magnifying glass or press the ENTER key on your keyboard to validate the entry.</p>
	<p>The software will then display the researched patient, or indicate that he is not part of the patient list.</p>

3.1.1.3. Modify/delete a patient file







	<p>Hover the mouse cursor over one of the patient files to reveal two additional icons.</p>
	<p>Click on the «information» icon to modify certain patient data (name, age, etc.).</p>
	<p>Click on  once the information has been modified or completed to save the changes.</p>
	<p>Click on the trash can, then validate the choice to delete a patient from the list.</p>

3.1.2. Patient interface (Dentist account)

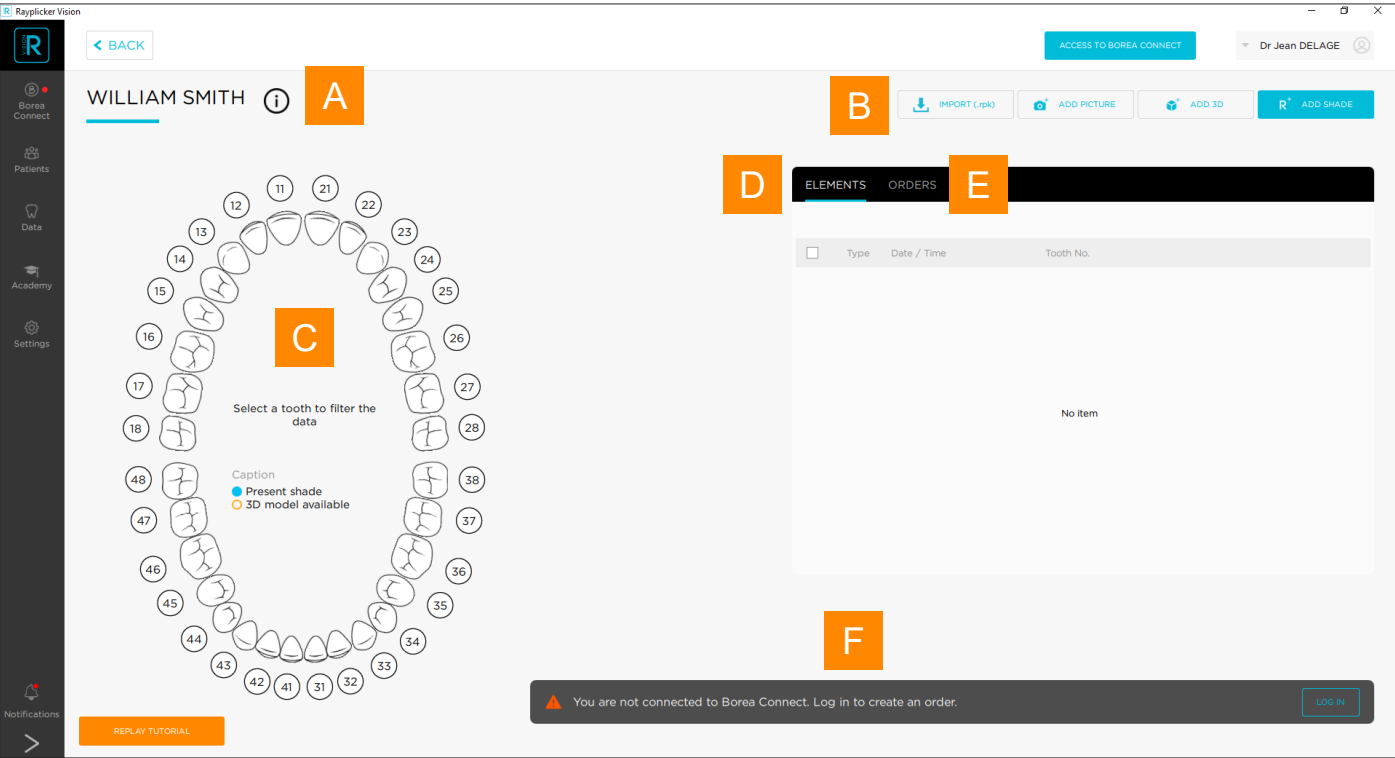

The patient interface looks like above, and is made up of various elements.

	The patient's name is displayed at the top left, click on the information icon to modify it.
	Here are indicated the different actions of the patient interface.
	Gives the possibility to add to the list of elements a shade file coming directly from a Rayplicker Handy device.
	Add shade taking files in the native format (.rpk) coming from the computer.

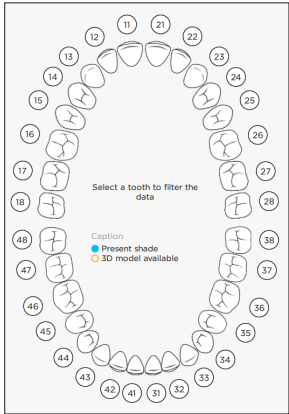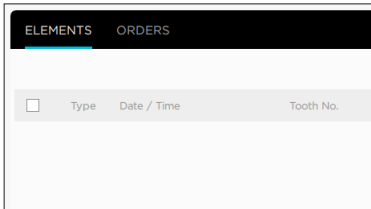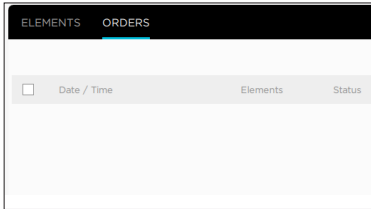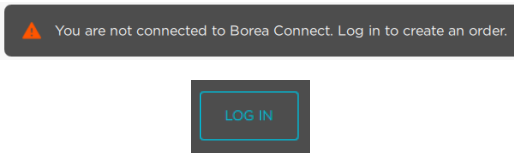B		Allows to add patient photos to a patient folder via the “Pics app solution” smartphone application or from the computer.
B		Allows to add a 3D file of .stl, .obj and .ply type from the computer.
C		This dental diagram makes it possible to visualize for which tooth(s) files are available, and to sort them by tooth number.
D		Under the «ELEMENTS» tab on the right of the screen are the different files available for the patient (shade, 3D, patient photo). Three options are available : compare shade files, export files, create an order.
E		The «ORDERS» tab gives you an overview of the different orders already established for this patient, with the possibility of viewing them in detail, or of deleting them.
F		Click on «LOG IN» to connect the Raypicker Vision software to the Borea Connect account.

3.1.2.1. Add a file to the Patient Interface

3.1.2.1.1. Add a shade

Adding a shade to your list of items can be done in two different ways, depending on where the file is coming from: a Rayplicker device or from the computer.

ADD A SHADE FROM RAYPLICKER DEVICE

IMPORT SHADES

CONNECTED DEVICES

RAYPLICKER

RAYPLICKER - Shades

Device users

All users

<input type="checkbox"/>	Date / Time	Patient name	Tooth No.
<input type="checkbox"/>	14/01/2022 - 16:11	Helen brook	11
<input checked="" type="checkbox"/>	11/01/2022 - 15:26	William smith	21
<input checked="" type="checkbox"/>	14/01/2022 - 16:13	William smith	22

Remove selected shades

IMPORT

Tips

Import a shade taking file

Return to the device's home page (screen with icons) and position the device on its base. Then, select the detected device or refresh the window.

FIND OUT MORE

Using a Rayplicker Handy: after taking the shade on a patient (see RAYPLICKER HAN-DY USER MANUAL) and connecting the base of y the device to the computer via the USB cable, click on **R+ ADD SHADE** then choose the file(s) to add to the list of elements then click on **IMPORT**

WILLIAM SMITH

SELECT A TOOTH TO FILTER THE DATA

SELECT

Present shade

3D model available

ELEMENTS

ORDERS

<input type="checkbox"/>	Type	Date / Time	Tooth No.
<input type="checkbox"/>	R	14/01/2022 - 16:13	21
<input type="checkbox"/>	R	14/01/2022 - 16:13	22

The imported shades appear in the right part of the patient interface under the «ELEMENTS» tab.

If the tooth number had been specified on the device, the imported shades are automatically indicated in blue on the corresponding tooth numbers on the dental diagram on the left side of the interface.

ELEMENTS

ORDERS

<input type="checkbox"/>	Type	Date / Time	Tooth No.
<input type="checkbox"/>	R	14/01/2022 - 16:57	<div><div>⚠</div><div>--</div></div>

SHADE VIEWER

Smith William

Created on 14/01/2022, 16:57

Tooth No.

⚠

--

Display shades

☐

TOOTH OUTLINE

STRATIFICATION

TRANSLUCENCY


If no tooth number has been specified on the device, it can be indicated it in the «ELEMENTS» section or directly from the «SHADE VIEWER» window that appears on the screen following import.

21

ADD A SHADE FROM THE COMPUTER OR NETWORK




Click on «import» from the patient folder.

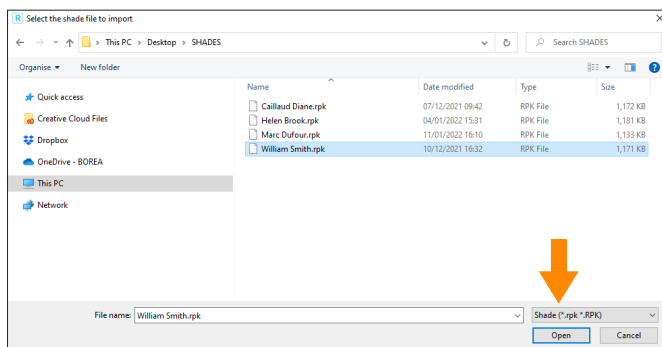


Select the shade file (.rpk) from the computer explorer and click on «Open».


3.1.2.1.2. Import a 3D file



Click on «ADD 3D» to import a 3D file of (.stl), (.obj) and (.ply) type from the computer.

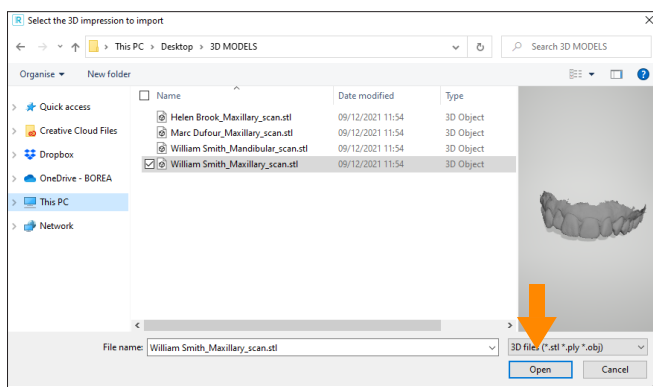


Select the 3D file from the explorer and click on «Open»

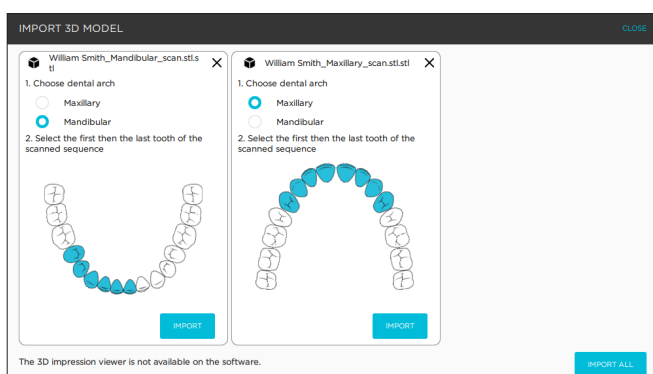


Indicate whether it is the mandible and/or the maxillary, then select the concerned teeth.





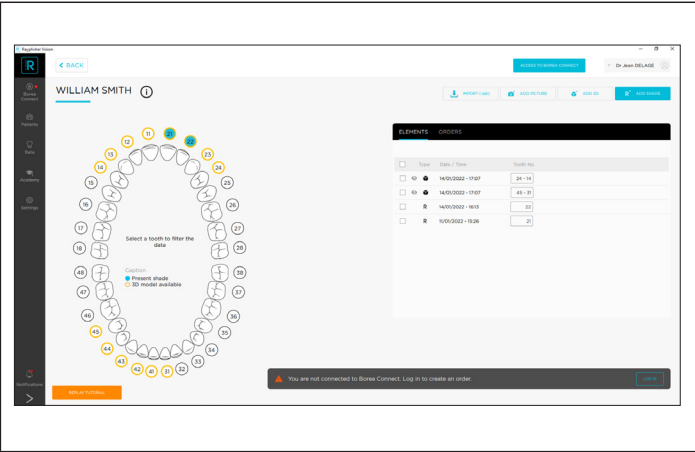


Click on **IMPORT** or **IMPORT ALL** to import the files into the patient folder.


	<p>Once the 3D file has been imported, it appears on the right in the “ELEMENTS” section of the patient interface and in yellow on the dental diagram.</p>
--	--

3.1.2.1.3. Import a patient picture

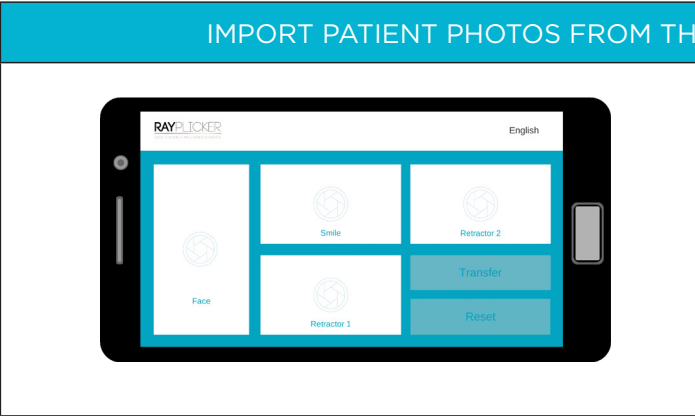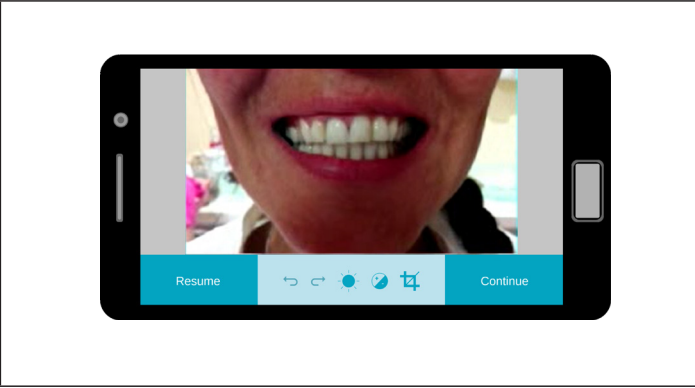The tool  allows to add photos of the patient’s face or smile to the patient folder and then to the order, in order to give to the dental technician a better idea of the context.


Two ways of doing this are suggested: either by importing a photo previously saved on the computer, or by using the Borea smartphone application “Rayplicker Pics App Solution”, which can be downloaded from the App Store and Google Play online stores.

IMPORT PATIENT PHOTOS FROM THE RAYPLICKER PICS APP SOLUTION	
	<p>Once downloaded and opened, the application suggest to take 4 photos:</p> <ul style="list-style-type: none">*Face*Smile*Retractor 1 and 2
	<p>Once photo has been taken, various tools allow to modify it:</p> <ul style="list-style-type: none"> Cancel Restore Luminosity Contrast Cropping

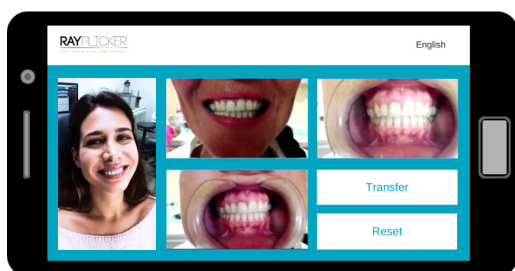


After taking the photos, click «Transfer» to go to the next step.

Click on «Reset» to erase the photos.

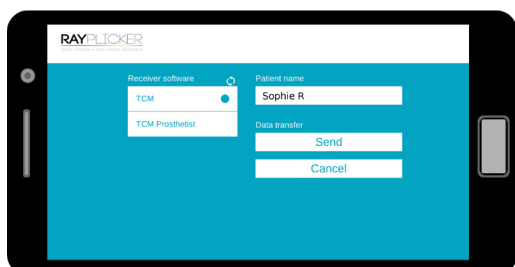


Complete the patient's name.
Search for software by clicking on the arrow.

Select the software that will receive the data then click on send.

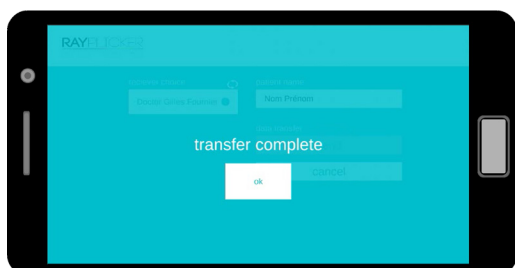


The photos will be automatically transferred by wifi to the Rayplicker software.


*Important: make sure that both devices (Phone/tablet as well as the computer) are connected to the same wifi network. It will also be necessary to have launched the Rayplicker Vision software on the computer.





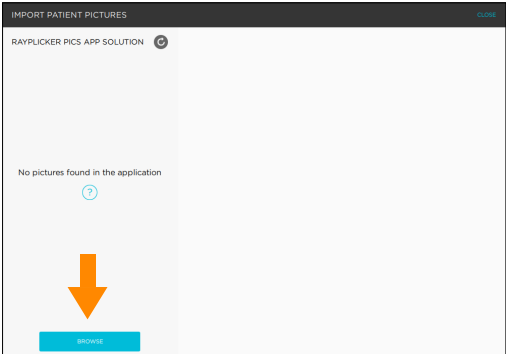
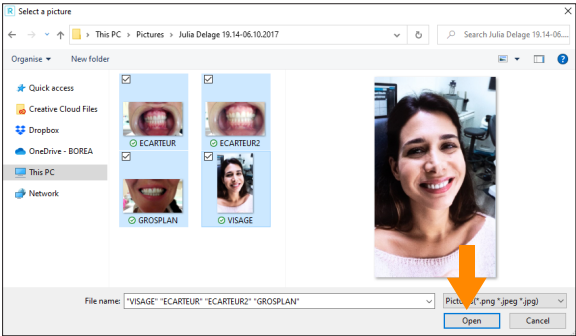
On the Vision software, click on «ADD PICTURE» to open the interface below.

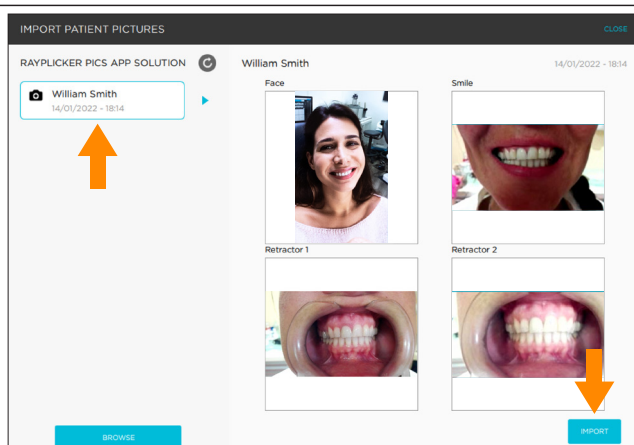


Choose the patient's photo folder on the left. Click on «IMPORT».

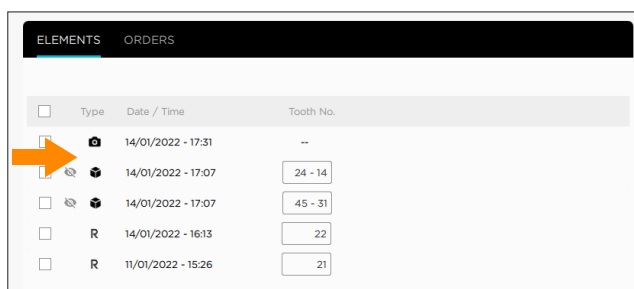

The photos recognizable by the icon  are then added to the list of “ELEMENTS”.

IMPORT PATIENT PHOTOS FROM THE COMPUTER	
	To import a patient photo from the computer, click on «ADD PICTURE».
	Click on «Browse».
	The explorer opens and gives the possibility to search on the computer, select the chosen file and click on open. .

3.1.2.2. Selection via dental chart

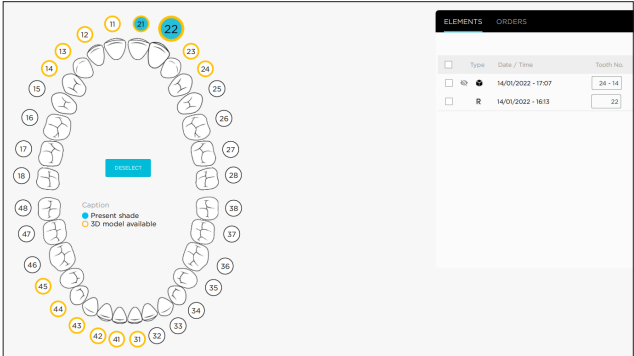
	<p>This diagram of the maxilla and mandible allows to filter the available elements (shade(s), patient photo(s), 3D file, pdf files) for a tooth.</p> <p>To filter, click on one of the tooth, and under the «ELEMENTS» tab on the right of the screen will only appear the files linked to it. (Here tooth 22 has been selected)</p>
---	---

3.1.2.3. Items & Order Tabs

Under the Elements tab, the different files available for the patient appear. The type of item as well as the date and time of acquisition are indicated. It is possible to specify to which tooth number these files correspond to. Three tools are available:

- The shade comparator

The comparison tool enables comparative analyzes based on CIE L*a*b* values between two or three acquisitions. A comparative (or bleaching) report can also be generated and saved in (.pdf) format.

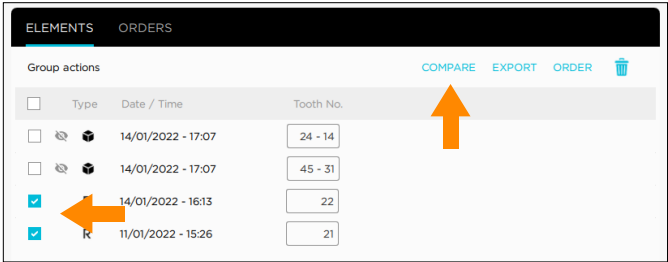


The screenshot shows a table with columns: Group actions, Type, Date / Time, and Tooth No. There are four rows of data. The first two rows have checkboxes that are not selected. The third and fourth rows have checkboxes that are selected. An orange arrow points to the 'COMPARE' button in the top right corner of the table area.

To launch the comparator window, select two shades by checking their box then click on «COMPARE».

Two comparisons are indicated: Visual and Shade.


Visual comparator:



The screenshot shows a close-up of a tooth. A vertical white line is drawn down the center of the tooth. A double-headed arrow is positioned on the line, indicating that the user can move the cursor to compare different parts of the tooth.

Use the mouse to move the cursor to the right or to the left.









Shade comparator:



The screenshot shows the 'SHADE COMPARATOR' window. It displays two tooth images side-by-side with color overlays. Below the images is a table with CIE L*a*b* values for three different acquisitions. The table has columns for 'Shade', 'L', 'a', 'b', and 'Delta' for each acquisition. The 'Delta' column shows the difference between the first and second acquisitions, and between the first and third acquisitions.

	14/01/2022 - 17:42	11/01/2022 - 15:26	Delta	14/01/2022 - 17:42	11/01/2022 - 15:26	Delta	14/01/2022 - 17:42	11/01/2022 - 15:26	Delta
Shade	2H2	1H2	-	2H1	1H1	-	1H1	1H1	-
L	76.2	77.4	1.2	79.2	78.8	-0.4	68.0	67.9	-0.1
a	4.5	2.7	-1.8	1.2	0.3	-0.8	0.3	0.1	-0.2
b	17.3	16.2	-1.1	10.4	11.1	0.7	6.8	7.4	0.6
			ΔE = 1.9			ΔE = 1.0			ΔE = 0.5

Compare multiple shade files based on multiple shade-guide references and CIE L*a*b* values.

	<div> Single area</div> <div> Oval multi-areas</div> <div> Rectangular multi-areas</div>	Select the number (1 or 3) and shape (oval or rectangle) of areas desired for analysis.
<div></div> <div></div>	The padlock is used to freeze the movement of the analysis area.	
<div></div> <div></div>	Allows to reduce or increase the size of the analysis area.	

Generate a report:

After performing the color analysis, a report can be generated in .pdf format by clicking on

CREATE REPORT (.pdf)

A comparative report or a bleaching report can be edited. The bleaching report is generated when the Vita Bleachguide 3D Master® shade guide is selected.

RAYPLICKER VISION

DR JEAN DELAGE
6 Allée Duke Ellington
87200 Limoges
098372181
jd.croire@korea-dental.com

SHADE COMPARISON REPORT
14/01/2022

PATIENT
WILLIAM SMITH, Male, 54 years old

SHADE GUIDE
Vita 3D Master

14 January 2022 / 14 January 2022

	14/01/2022			14/01/2022			14/01/2022			14/01/2022		
	2002	3002	4002	2002	3002	4002	2002	3002	4002	2002	3002	4002
L	76.2	71.4	1.2	76.2	70.8	4.4	68.0	67.9	4.1			
a	4.3	2.7	1.6	1.2	0.5	-0.0	0.3	0.1	-0.2			
b	17.8	18.2	-0.4	10.4	11.1	0.7	8.8	7.4	0.8			

ΔE = 1.9 ΔE = 1.9 ΔE = 0.5

Here an example of a comparative report between two shade files according to VITA Toothguide 3D-MASTER® reference.

RAYPLICKER VISION

DR JEAN DELAGE
6 Allée Duke Ellington
87200 Limoges
098372181
jd.croire@korea-dental.com

BLEACHING REPORT
14/01/2022

PATIENT
WILLIAM SMITH, Male, 54 years old



SHADE GUIDE
Vita Bleachguide 3D Master

14 January 2022 14 January 2022

Example of a first page of a bleaching report.


- Export



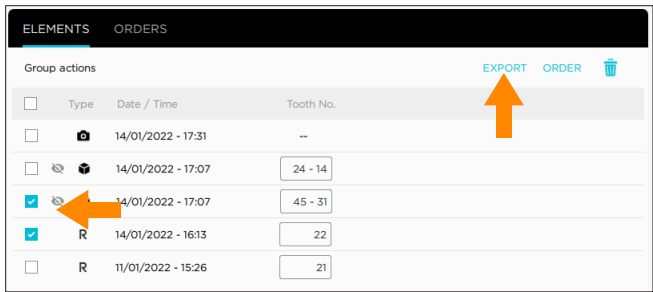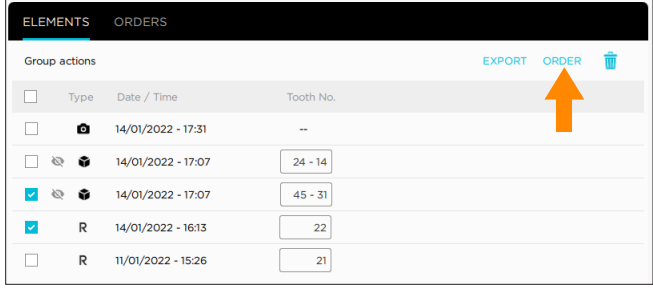



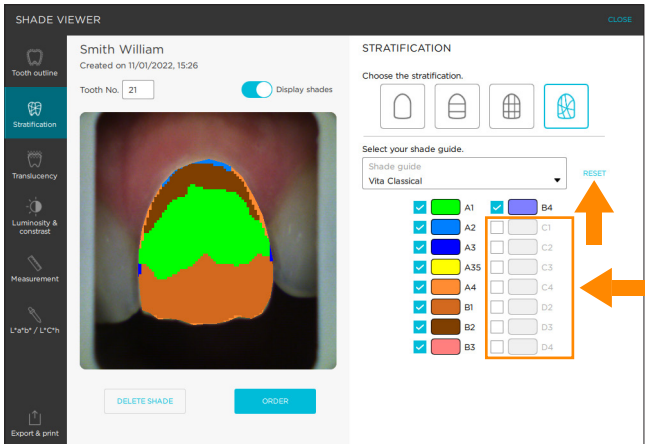
To keep a file (Shade, 3D or photo), select the desired file(s) then click on to choose the target folder on the computer.

	<p>To keep a file (Shade, 3D or photo), select the desired file(s) then click on to choose the target folder on the computer.</p>
	<p>Finally, check one or more files then click on «ORDER» to add them to the order. See «3.1.4. Create an order (Dentist account)», page 32»</p>

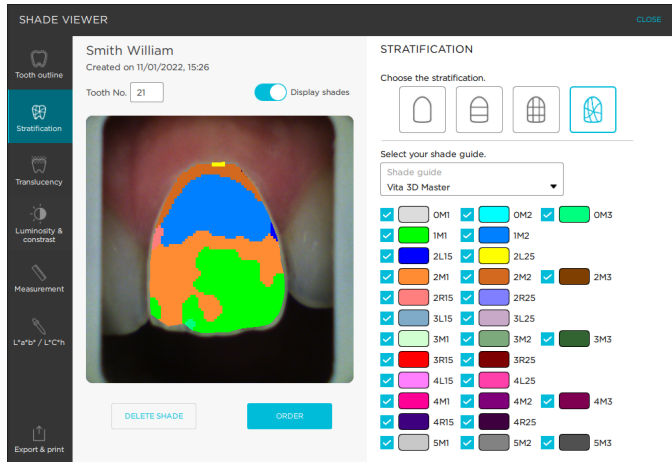
3.1.3. Shade viewer

Among elements, click on a shade **R** to open the shade viewer and its various tools, accessible via the tabs on the left.

The Stratification tab	
	<p>The Stratification tab gives the possibility to view the shade acquisition made under several level of detail.</p>

<p>Choose the stratification.</p> 	<p>Click on the pictogram corresponding to the desired level of stratification:</p> <ul style="list-style-type: none">  Overall shade  3 parts shade  9 parts shade  Detailed mapping
	<p>Select or unselect «Display shades» to display the polarised image of the tooth.</p>
<p>Select your shade guide.</p> <div data-bbox="280 1218 622 1281"> Shade guide Vita 3D Master </div>	<p>Choose the reference shade guide in the library list. here below are the available shade-guides:</p> <ul style="list-style-type: none"> • VITA 3D-MASTER® • VITA Classical A1-D4® • VITA Classical A1-D4® + Bleached Shades • Ivoclar Chromascop • Shofu Vintage • Noritake
	<p>Customize a shade guide by selecting or un-selecting shades.</p> <p>Only the selected shades will be used for the shade analysis.</p> <p>Click on «RESET» to come back to standard configuration.</p> <p>Here in the example, C & D shades have been unselected from the VITA classical A1-D4® shade guide.</p>


The tooth outline tab

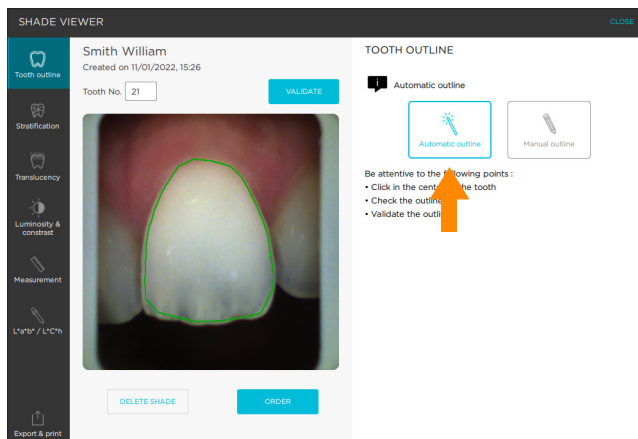


The tooth outline tab allows to redefine the contour of the tooth.

Click on automatic contouring then on the tooth so that the software creates the contour automatically.

If the contour is correct, click on Validate.

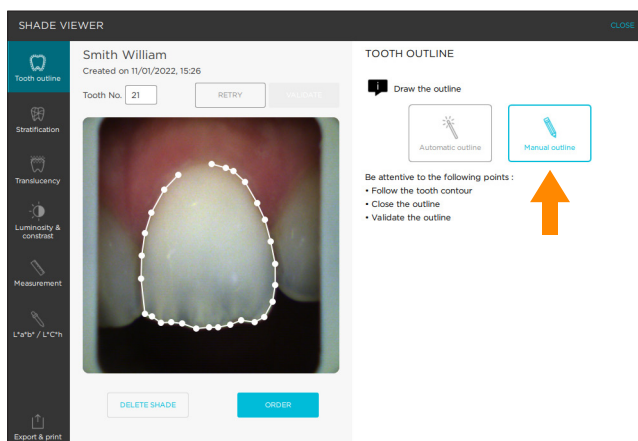


If the outline does not conform, click on manual trimming to redefine it, point by point.

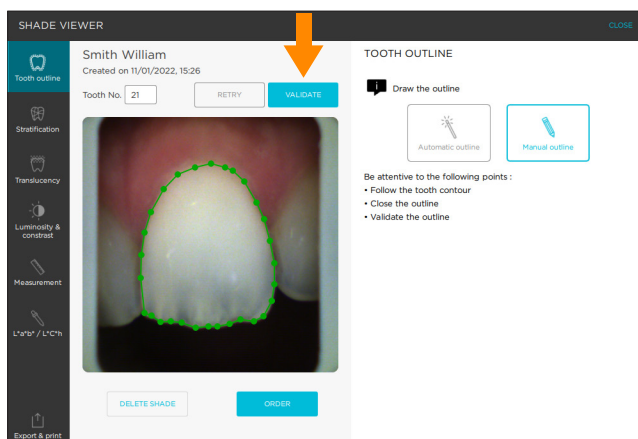

Finish the outline by clicking on the starting point. When the outline is green, click on Validate to confirm.

The translucency tab

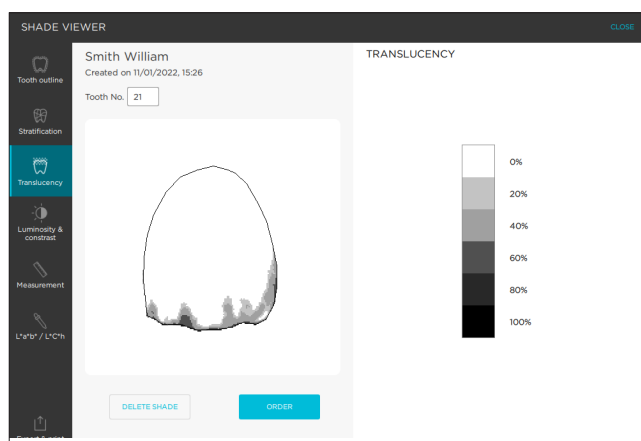


The Translucency tool allows to view a map of the translucency of the tooth.

The level of translucency is readable by a gray scale indicating the presence of translucency on a scale of 0% to 100%.

0% being non translucent
100% being the most translucent

Luminosity & contrast tab

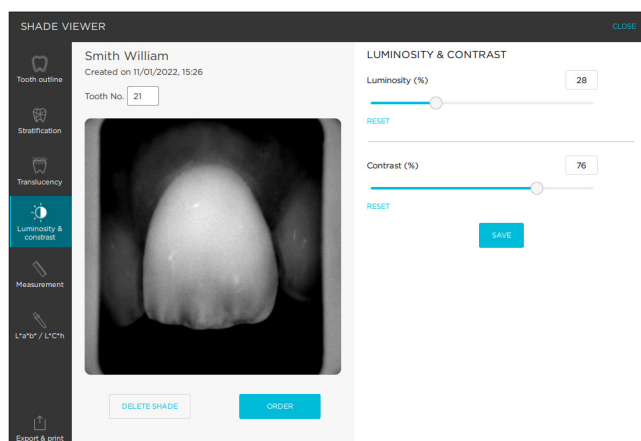


This black and white adjustment tool converts color polarized photo to grayscale.

Use the sliders to modify the brightness and contrast parameters and thus bring out the distribution of dentin, enamel, or other remarkable characteristics.


Click on “save” to save the configuration.

Measurement tab

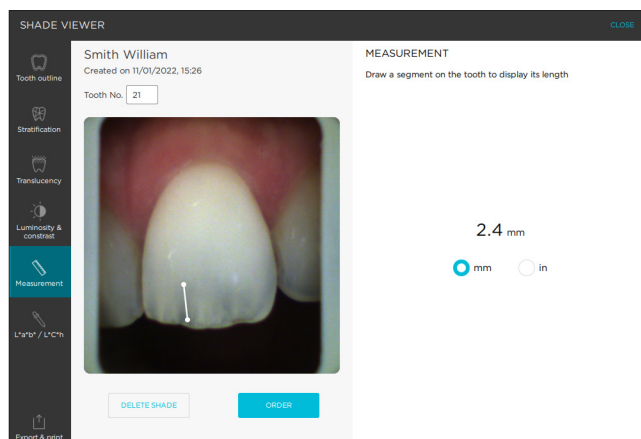

This measurement tool makes it possible to locate and measure the location of remarkable areas such as areas of translucency or other remarkable characteristics (spots, slits).

L*a*b* / L*C*h tab

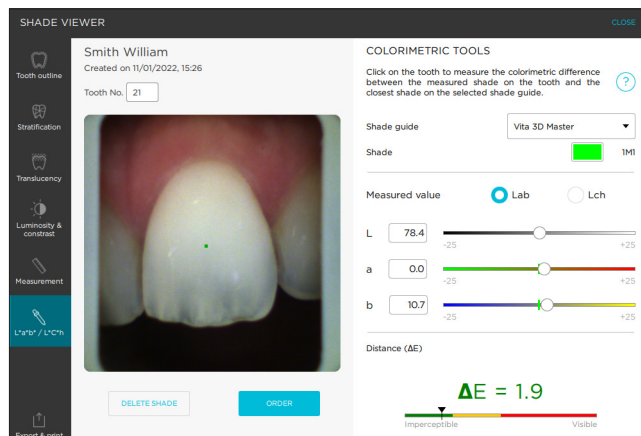


Calculate the “Delta E or ΔE ” colorimetric difference between the actual shade of the tooth and the closest shade according to the selected reference shade guide.

Visualize the differences according to the 3 dimensions of color: luminosity, saturation and hue.

This analysis can be carried out under the Cie L*a*b* or L*C*h repository.

Determine by groups of 4x4 pixels the colorimetric coordinates by clicking on a point of the tooth. You can also access this same information but for a larger area by clicking and dragging your mouse over the part to be analyzed.

Export tab

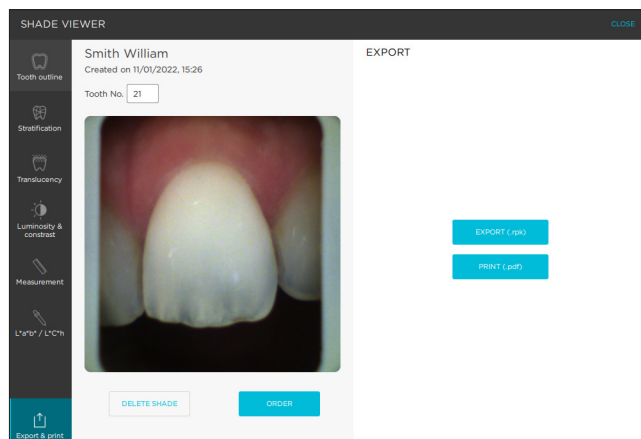

Export shade analysis in a simplified .pdf format to send the order form by e-mail, or in .rpk format to have the possibility of later accessing all the information.

Print the simplified version directly by clicking on the button provided for this purpose.

Finally, click on «ORDER» to add this shade to your Borea Connect account, after indicating the tooth number.

3.1.4. Create an order (Dentist account)


You have various options for sending an order form to your laboratory. Indeed, an order can be created on three different interfaces if the software is connected to the Borea connect.

Via the list of items from the patient folder.
«ORDER» button is displayed on the subject
line.



ORDER

3.2. The workflow per data


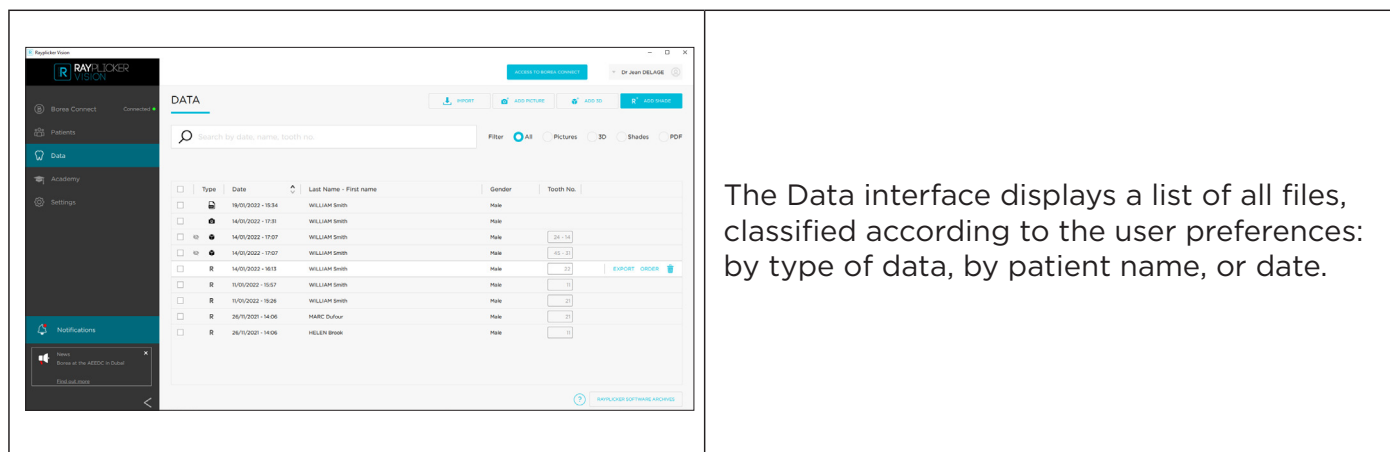





3.2.1. Add a data (Dentist account)

To add data to the data list, click on one of the import buttons located at the top right of the screen:



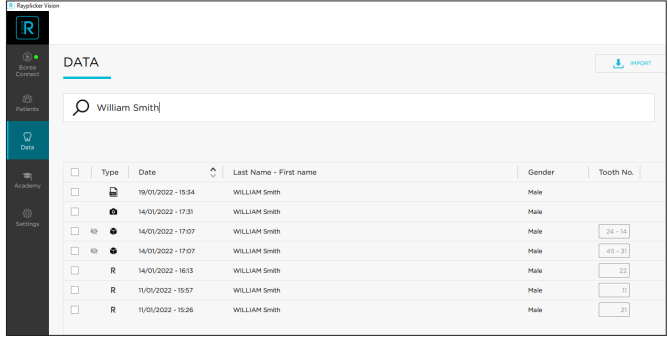
	Provides the ability to add a shade directly from a Rayplicker Handy device to the data list.
	Add a shade file (.rpk) from the computer to the data list.
	Allows to add context photos to the order form, via the Rayplicker Smartphone application or from the computer.
	Import a 3D file of type .stl, .obj and .ply from the computer.

3.2.1 Filter / Consult data

Filter the files by type (shade , patient photo , 3D file  or .pdf file ) by clicking on the button provided for this purpose:



A search function by patient is present in the upper part.





	<p>Click on the search text field. Enter the patient's name or social security number.</p>
	<p>Click on the magnifying glass or press the ENTER key on your keyboard to validate the entry.</p>
	<p>The software will then display the patient , or indicate that he is not part of the data list.</p>

To consult a data, click on it.

- For a shade  please refer to part «3.1.3. Shade viewer», page 27.

3.2.3. Manage data

Different actions are possible by clicking on the corresponding icon:

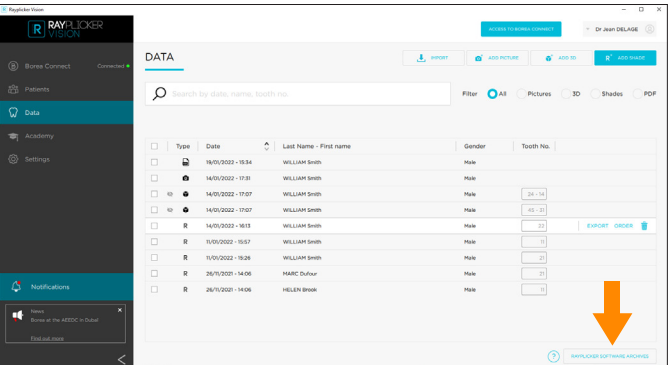


	<ul style="list-style-type: none"> - Export a file: EXPORT - Order a file: ORDER - Delete a file: 
	<p>For users of the previous Rayplicker software, an access to old archives is possible by clicking on :</p> 

4. REGISTRATION & OVERVIEW OF BOREA CONNECT

Borea Connect is a connected and secure portal aimed at facilitating data sharing between the dental practice and the dental laboratory. It makes it possible to produce and then send via Cloud a prosthesis order by attaching several types of files: shade file(s), 3D models, patient photo(s), and by providing a certain amount of information on the product ordered (type of prosthesis, desired level of detail for shade, occlusion, etc.). The prosthetist thus has the possibility of receiving most of the information provided by the Rayplicker Handy device, without having to go through the Rayplicker Vision software. Then, chat via the messaging system to add details, keep informed of the progress of the work...


4.1. Account creation






The gateway between the «ORDER» feature of Rayplicker Vision and Borea Connect is automatic and leads directly to the registered dentist account. It is also possible to connect to it via an Internet browser at the following address: <https://borea-connect.com/user/signin>

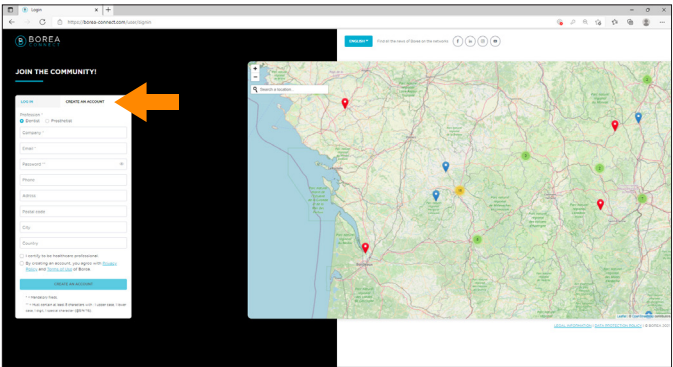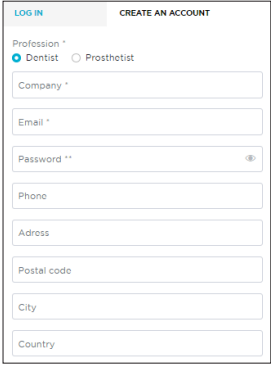


	<p>Once on the home page, click on</p> <div style="border: 1px solid #ccc; padding: 5px; display: inline-block; background-color: #f0f0f0;"> CREATE AN ACCOUNT </div>
	<p>Continue the registration by indicating the type of account to create (dentist or prosthetist), name and first name, an email address and an associated password.</p> <p>Optional fields like address and phone number can be filled in.</p>
<p><input type="checkbox"/> I certify to be healthcare professional.</p> <p><input type="checkbox"/> By creating an account, you agree with Privacy Policy and Terms of Use of Borea.</p>	<p>Confirm that you are a healthcare professional and agree to the privacy policy and terms of use. Finally, validate the creation of the account by clicking on :</p> <div style="border: 1px solid #00a0e3; padding: 5px; display: inline-block; background-color: #00a0e3; color: white;"> CREATE AN ACCOUNT </div>
	<p>The creation of the account must be confirmed by clicking on the link received by email to the email address previously used for the creation of the account.</p>

4.2. Dashboard

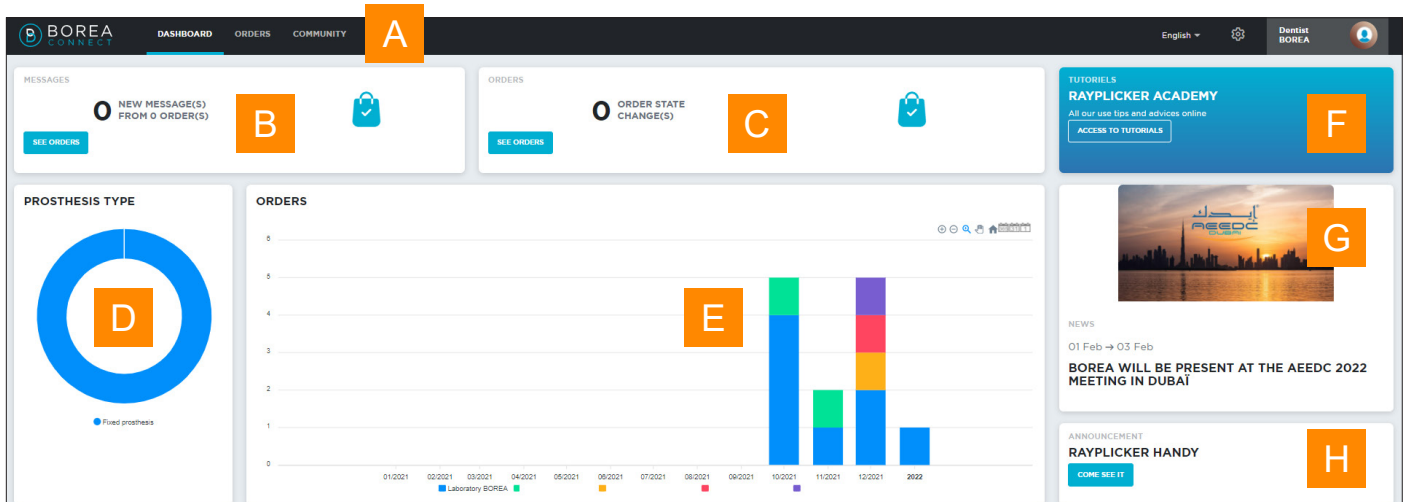
Once registered, the dashboard is displayed with several information available :

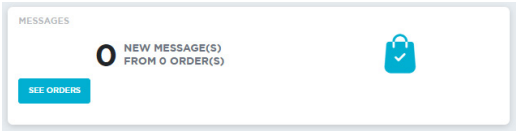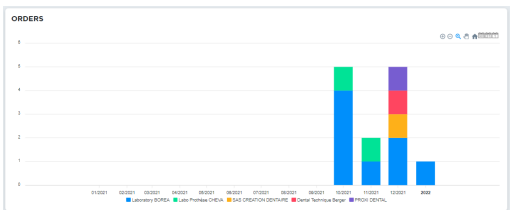

<p>A</p> 	<p>The upper taskbar gives access to the different features/tools of Borea Connect: the dashboard, the orders, the Rayplicker community, the settings.</p>
<p>B</p> 	<p>The most recent notification appears here. Click on it to read it, and access other notifications.</p>
<p>C</p> 	<p>Quick information about the latest orders is displayed here. Click on SEE ORDERS to access orders.</p>
<p>D</p> 	<p>This statistical part of the dashboard shows what type of prostheses have been ordered over a predefined period.</p>
<p>E</p> 	<p>Statistics always, with here an overview of the types of orders made over a given period.</p>

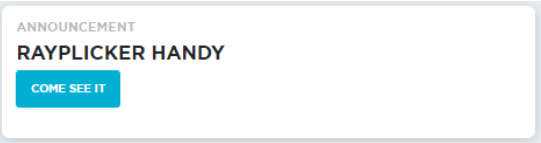

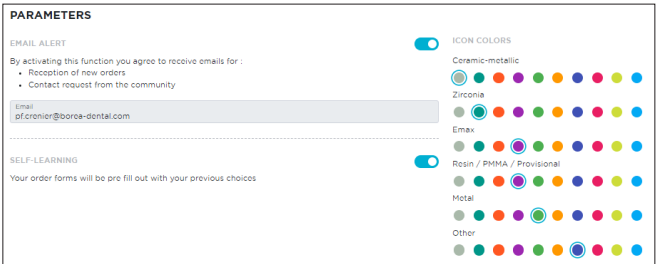

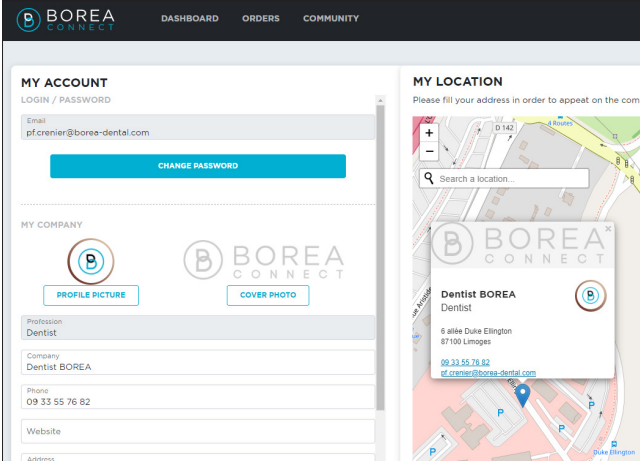

F	 <p>TUTORIELS RAYPLICKER ACADEMY All our use tips and advices online ACCESS TO TUTORIALS</p>	This field gives access to the «Academy» page from the Borea website. Many information concerning the solution are indicated here as tutorials for example.
G	 <p>NEWS 01 Feb → 03 Feb BOREA WILL BE PRESENT AT THE AEDC 2022 MEETING IN DUBAI</p>	Here are displayed some «news» about the company Borea.
H	 <p>ANNOUNCEMENT RAYPLICKER HANDY COME SEE IT</p>	Click here to have more information about Borea products.

4.3. The Raypicker community

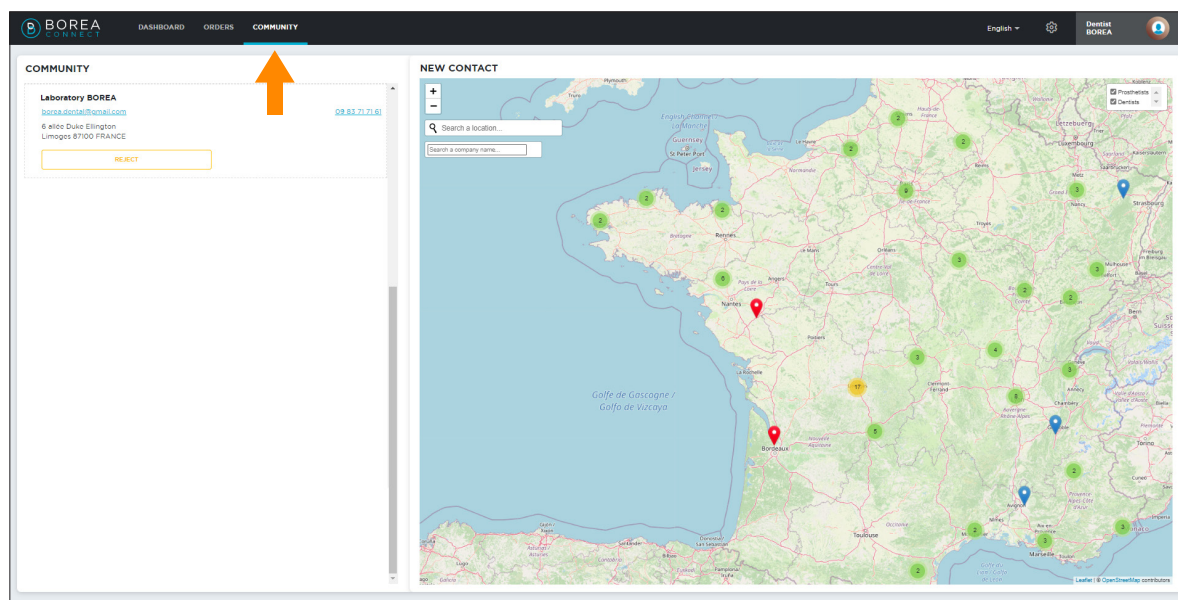

The Raypicker community is displayed on this page via a map showing the different users of the Borea connect platform. From this page, a dental surgeon have the possibility of sending a request for entering in contact with the laboratories geolocated on the map and then sending them prosthesis order.


4.4. Account settings

	<p>Clicking at the top right of the screen on the toothed wheel  gives access to various parameters.</p>
	<p>Activation or not of the email alert for new orders and contact request.</p> <p>Indication of the user email address.</p> <p>Activation or not of the self-learning function: if activated, the platform remembers user preferences when creating an order (type of order, prosthesis, shade guide, etc.).</p> <p>Configuration of order icons colors.</p>
	<p>The information initially entered on the Borea Connect home page (name, address, password, etc.) can be modified by accessing «My account».</p> <p>To do this, click at the top right of the screen on the user name of the Borea Connect account, then on click on «My Account».</p>
	<p>Click on  to modify the account password.</p> <p>Indicate and customise the account settings in «MY COMPANY».</p>

5. BOREA CONNECT - SEND AN ORDER

5.1. Finalize the order on Borea Connect

All orders, sent, processed, or still in draft form, are listed under the «ORDERS» tab. The last order transferred from the Vision software appears in draft format at the top of the list. Click on it to open it.

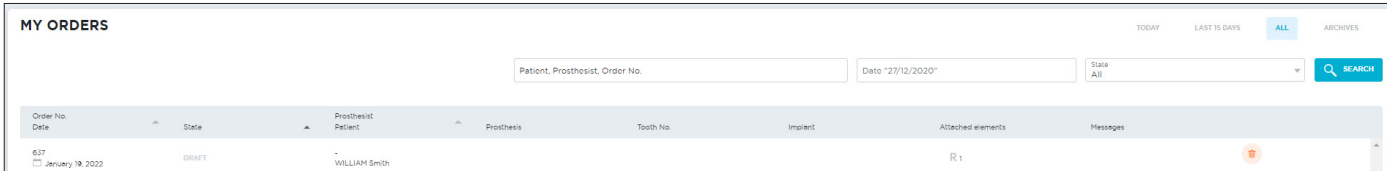

Order No	Date	State	Prosthesis	Patient	Prosthesis	Tooth No	Implant	Attached elements	Messages
617	January 19, 2022	DRAFT		WILLIAM Smith				R1	

Tip: once your Borea Connect account has been created, a simple click on «ORDER» on the Rayplicker Vision software will automatically open the draft!

Once opened, a few things must be filled in before it can be sent to the laboratory.

BOREA CONNECT DASHBOARD **ORDERS** COMMUNITY English Dentist BOREA

COMMAND 637

SMITH WILLIAM
Man, 55 years old

Attached elements
R 1

Comments

Delivery date
January 27, 2022

Recipient contact
Laboratory BOREA

SEND COMMAND

Command type
Fixed prosthesis

Prosthesis type
Colored Zirconia

ADDITIONAL INFORMATION

Pontic design

Occlusal
☒ Low ☐ Medium ☐ Hard

Occlusal contact
☒ Low ☐ Medium ☐ Hard

IMPLANTOLOGY

Implantology

Implant type

PRODUCTION TEETH

18 17 16 15 14 13 12 11 21 22 23 24 25 26 27 28
48 47 46 45 44 43 42 41 31 32 33 34 35 36 37 38

Create a unitary element : please select the production tooth/teeth ([simple click](#))

Create "an integral element" / "Bridge" : please select the first tooth of the "integral block" / "Bridge" ([double click](#)) then select the last tooth of this "block" / "Bridge" ([simple click](#))

Delete an item : [double click](#) on the item to delete

SHADE

Reference shade
shade 1

Translucency:
Neutral

Stratification

Low **Standard** High

Shade guide
Vita 3D Master

Impression

☒ Physical desinfected ☐ Physical undesinfected ☐ Digital Borea Connect ☐ Digital other

Attached elements

R

A

SMITH WILLIAM
Man, 55 years old

Comments

Delivery date
January 27, 2022

Recipient contact
Laboratory BOREA

SEND COMMAND

Write a comment about the order and define a desired date of delivery for the order. Then click on «recipient» contact to add the recipient laboratory of the order.

B

Command type
Fixed prosthesis

Prosthesis type
Colored Zirconia

Overview

Choose here the type of

- Order: fxd or removable
- prosthesis: Metal ceramic, Zirconia...
- etc.

<div data-bbox="124 141 183 201">C</div> <div data-bbox="124 219 783 286"> <p>▼ ADDITIONAL INFORMATION</p> <div> <div>Pontic design</div> <div> <div>Occlusal</div> <div> <input checked="" type="radio"/> Low <input type="radio"/> Medium <input type="radio"/> Hard </div> </div> <div> <div>Occlusal contact</div> <div> <input checked="" type="radio"/> Low <input type="radio"/> Medium <input type="radio"/> Hard </div> </div> </div> </div>	<p>Additional information on occlusion, contact points, etc. can be added.</p>
<div data-bbox="124 340 183 400">D</div> <div data-bbox="124 418 783 492"> <p>▼ IMPLANTOLOGY</p> <div> <div>Implantology</div> <div>Implant type</div> </div> </div>	<p>In the case of an implantology treatment, it may be interesting to indicate the type of abutment and implant.</p>
<div data-bbox="124 598 183 658">E</div> <div data-bbox="124 676 783 752"> <p>PRODUCTION TEETH</p> <div> <div> <div>16</div><div>17</div><div>18</div><div>19</div><div>20</div><div>21</div><div>22</div><div>23</div><div>24</div><div>25</div><div>26</div><div>27</div><div>28</div> </div> <div> <div>46</div><div>47</div><div>48</div><div>49</div><div>50</div><div>51</div><div>52</div><div>53</div><div>54</div><div>55</div><div>56</div><div>57</div><div>58</div> </div> </div> <p>Create a solitary element: choose select the production tooth/teeth (1-28/29-58)</p> <p>Create "an integral element" / "bridge": choose select the first tooth of the "bridge house" / "bridge" (16-20/46-50) then select the rest tooth of the "house" / "bridge" (21-28/51-58)</p> <p>Default on form: (21/49) as the first to device</p> </div>	<p>Choose the production tooth/teeth to be produced by the laboratory.</p>
<div data-bbox="124 822 183 882">F</div> <div data-bbox="124 900 783 1113"> <p>SHADE</p> <div> <div>Reference shade</div> <div>Shade 1</div> </div> <div> <div>Translucency</div> <div>Neutral</div> </div> <div> <div>Stratification</div> <div> <div>Low</div><div>Standard</div><div>High</div> </div> </div> <div> <div>Shade guide</div> <div>Vita 3D Master</div> </div> <div> <div>2M2</div><div>2R3</div><div>2M1</div> </div> </div>	<p>Define here which color will be the reference of the order (if several color files are attached to the order).</p> <p>Bring out more or less translucency.</p> <p>Define the desired level of detail via layering.</p> <p>Choose the reference shade guide.</p>
<div data-bbox="124 1207 183 1267">G</div> <div data-bbox="124 1285 783 1350"> <p>Impression</p> <div> <input type="radio"/> Physical disinfected <input type="radio"/> Physical undesinfected <input checked="" type="radio"/> Digital Borea Connect <input type="radio"/> Digital other </div> </div>	<p>Information about the type of dental impression link to this order can also be specified.</p>
<div data-bbox="124 1402 183 1462">H</div> <div data-bbox="204 1402 703 1630"> <p>Attached elements</p> <div> <div>R</div> <div></div> </div> </div>	<p>Click on the elements attached (shade files, patient photo, 3D files) to the order to see them in detail.</p>
<div data-bbox="140 1720 767 2067"> <p>BOREA CONNECT</p> <p>Missing needed form data</p> <p>BACK COMMAND 637</p> <p>SMITH WILLIAM</p> <p>Man, 55 years old</p> </div> <div data-bbox="140 1917 767 2067"> <p>BOREA CONNECT</p> <p>Missing production tooth/teeth to draw command.</p> <p>BACK COMMAND 637</p> <p>SMITH WILLIAM</p> <p>Man, 55 years old</p> </div>	<p>If the order form is incomplete, the order can't be sent to the laboratory. A red banner will appear on the header to indicates that information are missing.</p>

5.2. Send the order to the laboratory






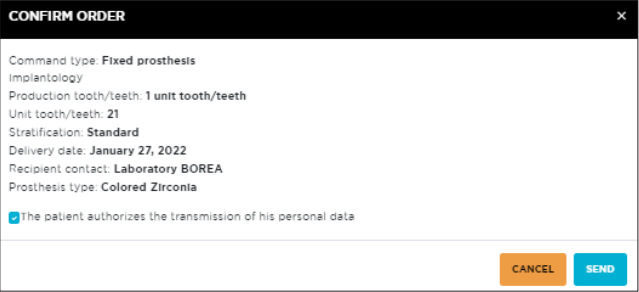
SMITH WILLIAM
 Man, 55 years old
 Comments

Attached elements
 R 1

Delivery date
 January 27, 2022

Recipient contact
 Laboratory BOREA

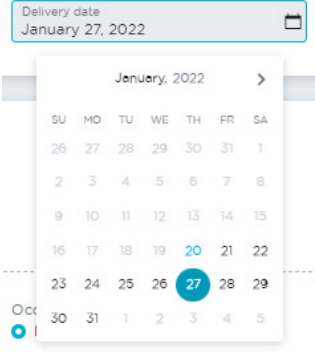
SEND COMMAND

	<p>The order is sent to the laboratory via the banner at the top of the screen. It is possible to attach a comment that the prosthetist will read, and to define a desired date of delivery for the prosthesis.</p>
	<p>Define a desired date of delivery for the order by using the calendar.</p>
	<p>Click on «recipient contact» to open your contact list and add the recipient laboratory of the order.</p> <p>If the contact list is empty, a contact request to a laboratory can be made from the «community» tab.</p> <p>Once the contact request is accepted, the laboratory will be add to the contact list.</p>
	<p>A .pdf order form can be generated by clicking on the «print» icon.</p>
	<p>Once the order fully completed, click on «send command».</p>
	<p>A summary of the order appears.</p> <p>Indicates if the patient authorizes the transmission of his personal data.</p> <p>Click on «SEND» for sending the order.</p> <p>Click on «CANCEL» to come back to the order page.</p>


6. RECEIVE THE ORDER AT THE LABORATORY

To create a Laboratory account on Borea Connect, see page «4.1. Account creation», page 35.

6.1. Receive the order via Borea Connect

	<p>If email notification is set up for a new order then, click on the link in the email to access the order on Borea Connect.</p> <p>Otherwise, log in to your Borea Connect account then access the list of orders received via the top banner (the last order received being displayed at the top of the list).</p>
---	---

6.1.1 Interpret the order

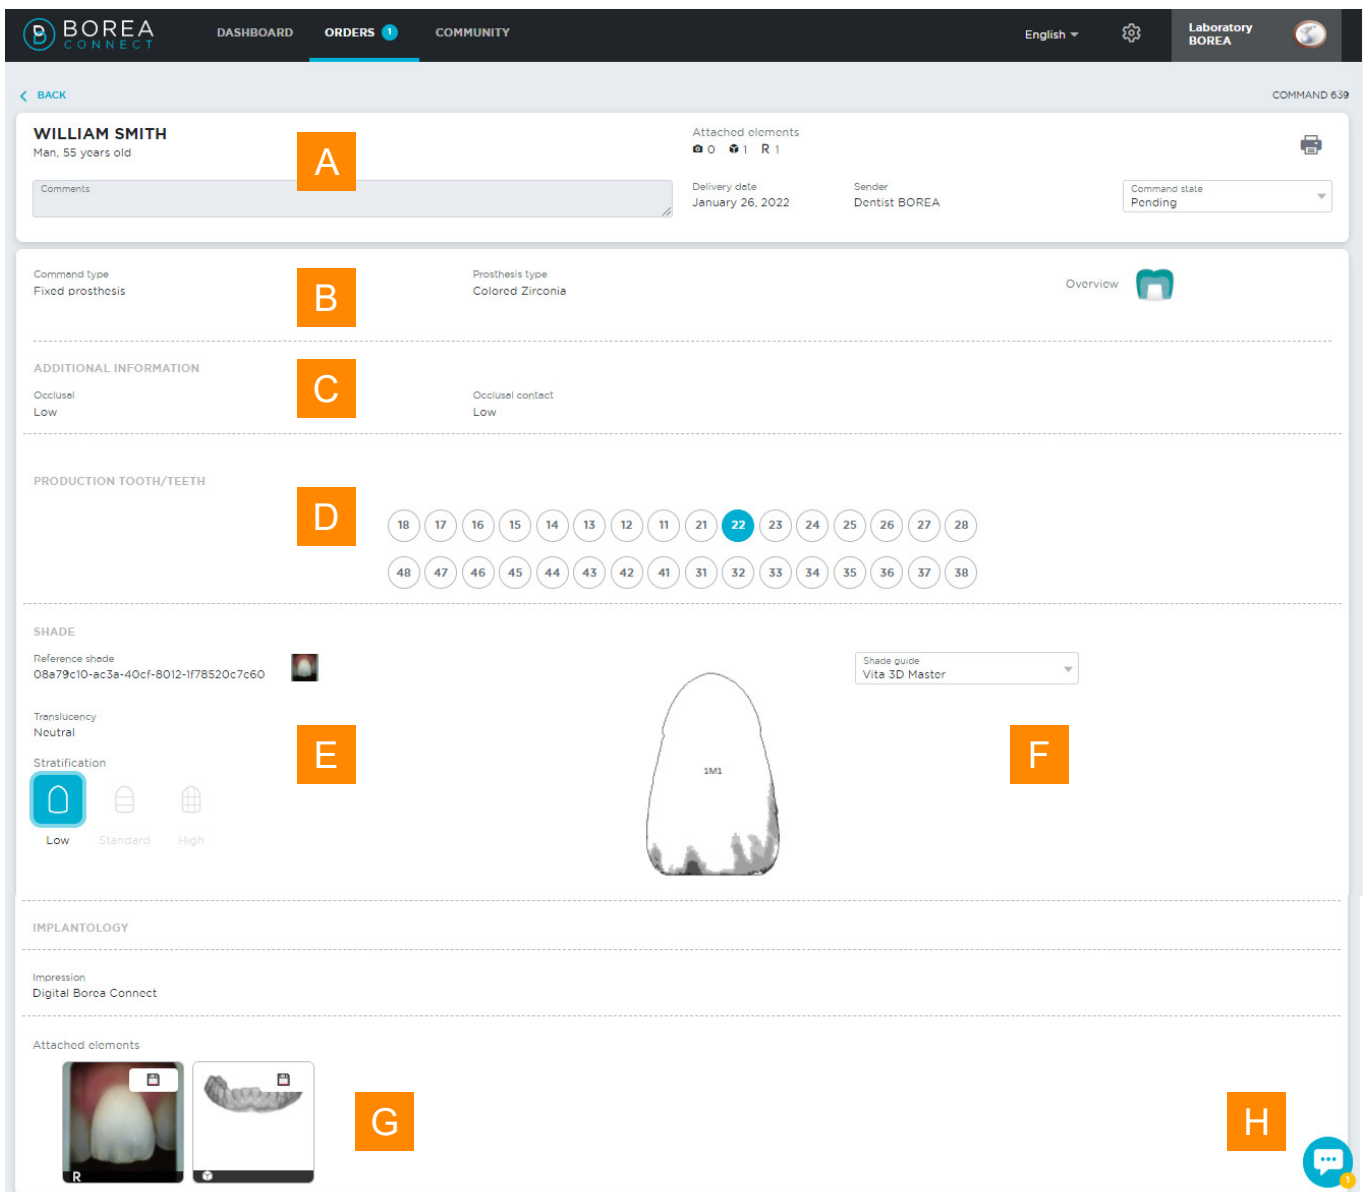

BOREA CONNECT DASHBOARD **ORDERS** 1 COMMUNITY English Laboratory BOREA

[BACK](#) COMMAND 639

WILLIAM SMITH
Man, 55 years old

Comments

Attached elements
0 0 1 R 1

Delivery date
January 26, 2022

Sender
Dentist BOREA

Command state
Pending

Command type
Fixed prosthesis

Prosthesis type
Colored Zirconia

Overview

ADDITIONAL INFORMATION

Occlusal
Low

Occlusal contact
Low

PRODUCTION TOOTH/TEETH

18 17 16 15 14 13 12 11 21 22 23 24 25 26 27 28
48 47 46 45 44 43 42 41 31 32 33 34 35 36 37 38

SHADE

Reference shade
08a79c10-ac3a-40cf-8012-1f78520c7c60

Shade guide
Vita 3D Master

Translucency
Neutral

Stratification
Low Standard High

1M1

IMPLANTOLOGY




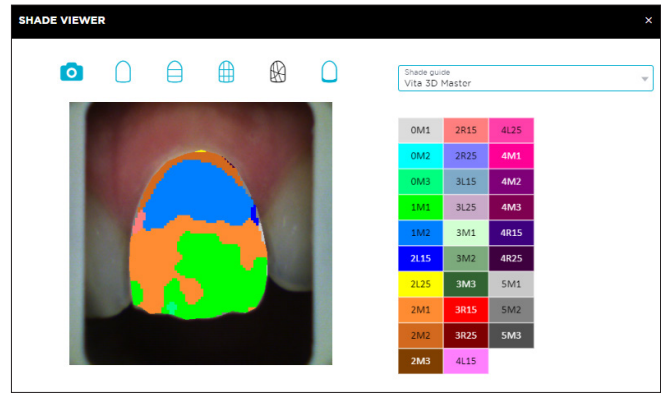
Impression
Digital Borea Connect



Attached elements

R



G

H
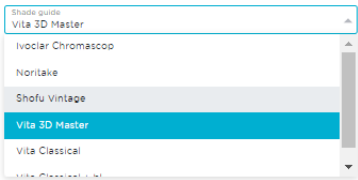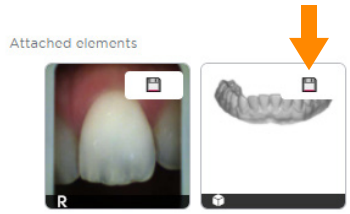
<p>A</p>	<p>The top banner shows a brief overview of the order: patient information, number of files attached to the order, delivery date desired by the customer, etc.</p>
<p>B</p>	<p>In the second part is information relating to the type of prosthesis to be made: command type (fixed prosthesis, removable, onlay, inlay), material (E-max, zirconia,...)</p>
<p>C</p>	<p>Additional information on occlusion, contact points, etc.</p>
<p>D</p>	<p>Tooth number to be manufactured.</p>
<p>E</p>	<p>The production tooth diagram tells you the level of detail desired by the practice in terms of the shade (1 global shade, 3 parts, 9 parts).</p>
<p>F</p> 	<p>Click here to see the tooth scheme according to an other shade guide reference.</p>
<p>G</p> 	<p>Files attached to the order can be saved by clicking on the icon  and opened by left clicking.</p>
<p>G</p> 	<p>Files attached to the order can be open by left clicking.</p> <p>Opening a shade file give access to a «SHADE VIEWER» window, where the tooth shade can be analysed under several mappings and shade references.</p> <p>Click on the last icon to display the translucency mapping.</p>

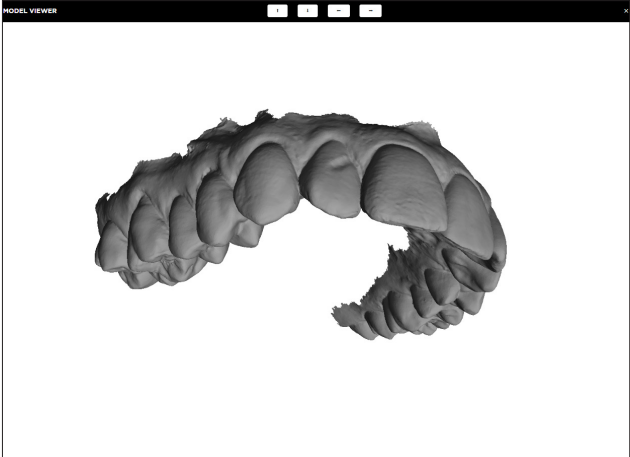
<div data-bbox="118 185 178 244" data-label="Text">G</div> 	<p>Opening a 3D file give access to a «MODEL VIEWER» window, where the 3D model can be visualize using the computer mouse and the icons on the top bar.</p>
<div data-bbox="118 786 178 844" data-label="Text">H</div> 	<p>Use this live chat to chat with the dental practice.</p>

6.1.2. Change order status / finalize order

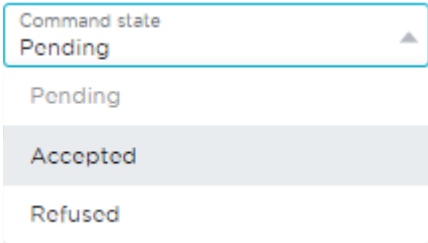





	<p>It is on the right part of the upper banner that orders can be accepted or refused. Once accepted, the statuts can be changed: in process, prosthesis sent, ended.</p>
	<p>An order remains accessible for 30 days from the date of import on the Borea connect by the practitioner. Then, the file is archived and a minimum of information rea-main accessible from the «ARCHIVES» filter.</p> <p>Borea recommends exporting the data in pdf or saving it on the Vision software for better traceability.</p>

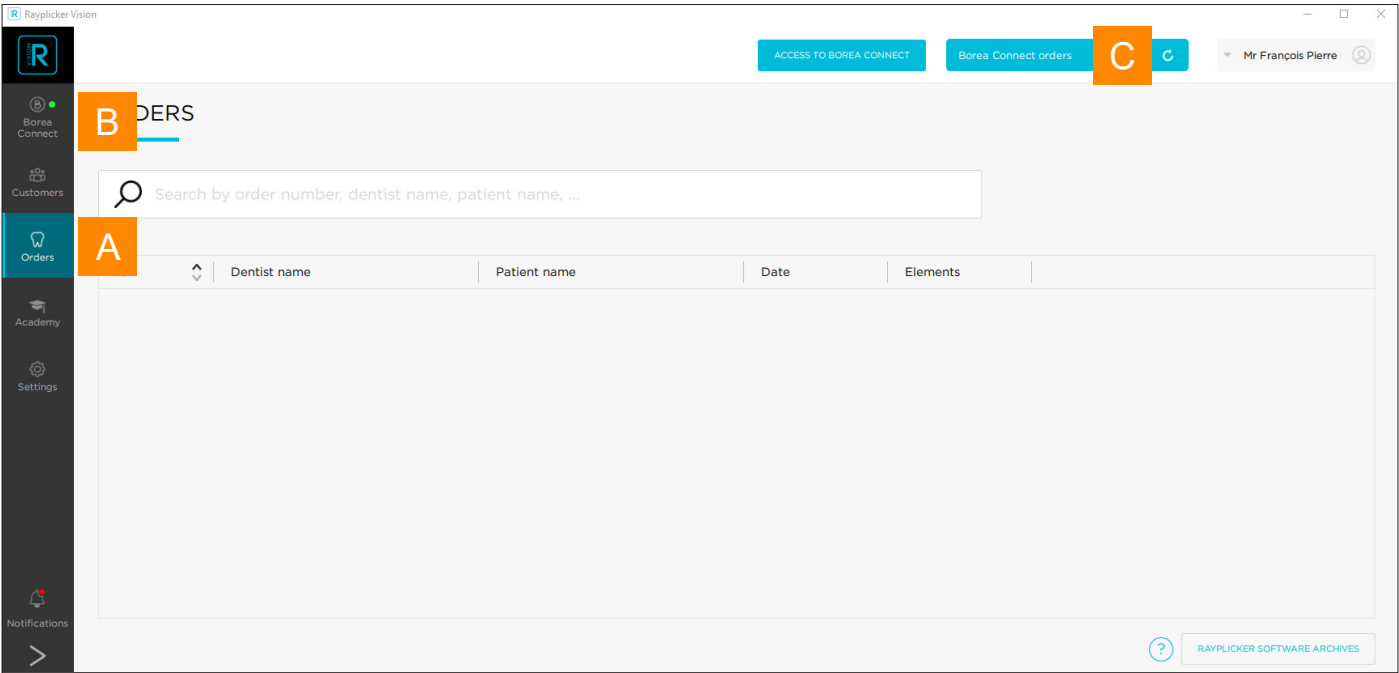6.2. Receive the order on the Raypicker Vision


6.2.1. Order tab



On the laboratory account, go to the «Orders» tab, log in to Borea Connect if it is not done yet. Then, click at the top right on «Borea Connect orders» to display the newly received orders. Then select the those to be imported and and click IMPORT.

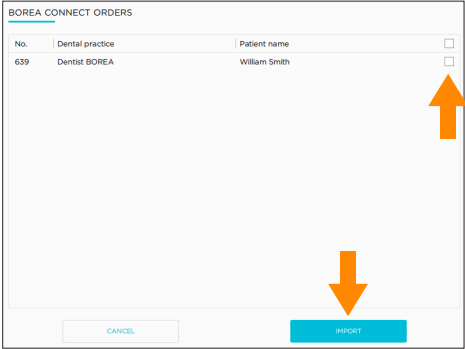	On your laboratory account, go to the ORDERS tab
	Log in to Borea Connect
	Click on «Borea connect orders» to open a new window that shows the orders received on the Borea Connect. 
	Select the order(s) and click on «IMPORT». 


When the downloaded order appears, it is indicated as «NEW».

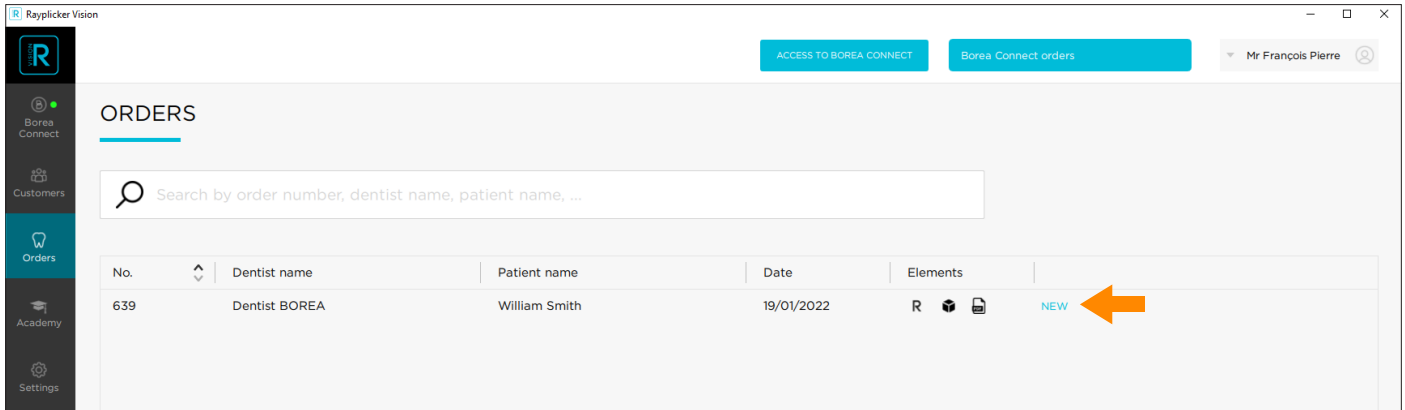

The screenshot shows the 'ORDERS' section of the Raypicker Vision interface. At the top, there are buttons for 'ACCESS TO BOREA CONNECT' and 'Borea Connect orders', and a user profile for 'Mr François Pierre'. Below these is a search bar with the placeholder text 'Search by order number, dentist name, patient name, ...'. The main part of the interface is a table with the following columns: No., Dentist name, Patient name, Date, Elements, and a status column. The first row of the table is highlighted in blue and has a 'NEW' label with an orange arrow pointing to it.

No.	Dentist name	Patient name	Date	Elements	
639	Dentist BOREA	William Smith	19/01/2022	R	NEW

Click on one of them to expand the list of available elements (shade, patient photo, 3D files, .pdf file), then on «OPEN» to view it. For a detailed explanation of the shade viewer: see [«3.1.3. Shade viewer», page 28](#)

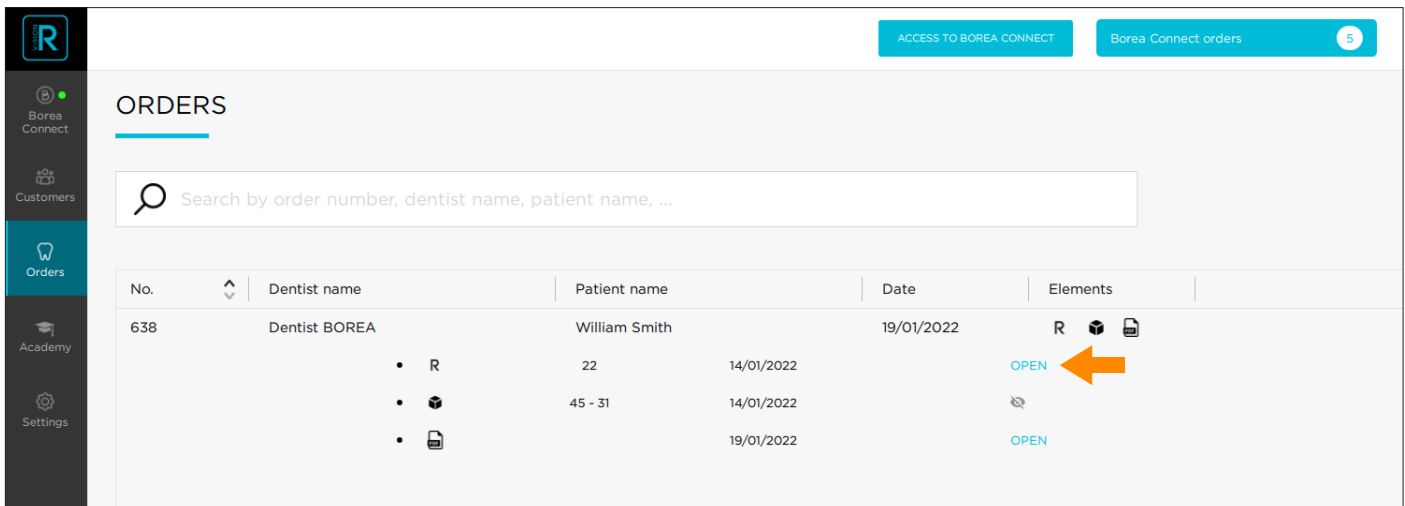


The screenshot shows the 'ORDERS' section of the Raypicker Vision interface, with the first row of the table expanded. The table has columns: No., Dentist name, Patient name, Date, Elements, and a status column. The first row (No. 638) is expanded to show a list of elements. The 'OPEN' button next to the first element is highlighted with an orange arrow.

No.	Dentist name	Patient name	Date	Elements	
638	Dentist BOREA	William Smith	19/01/2022	R	
				<ul style="list-style-type: none"> R 	
		22	14/01/2022		OPEN
		45 - 31	14/01/2022		
			19/01/2022		OPEN

6.2.2. Manage customers

As orders are received from practitioners, they will be added to the «Customers» tab.

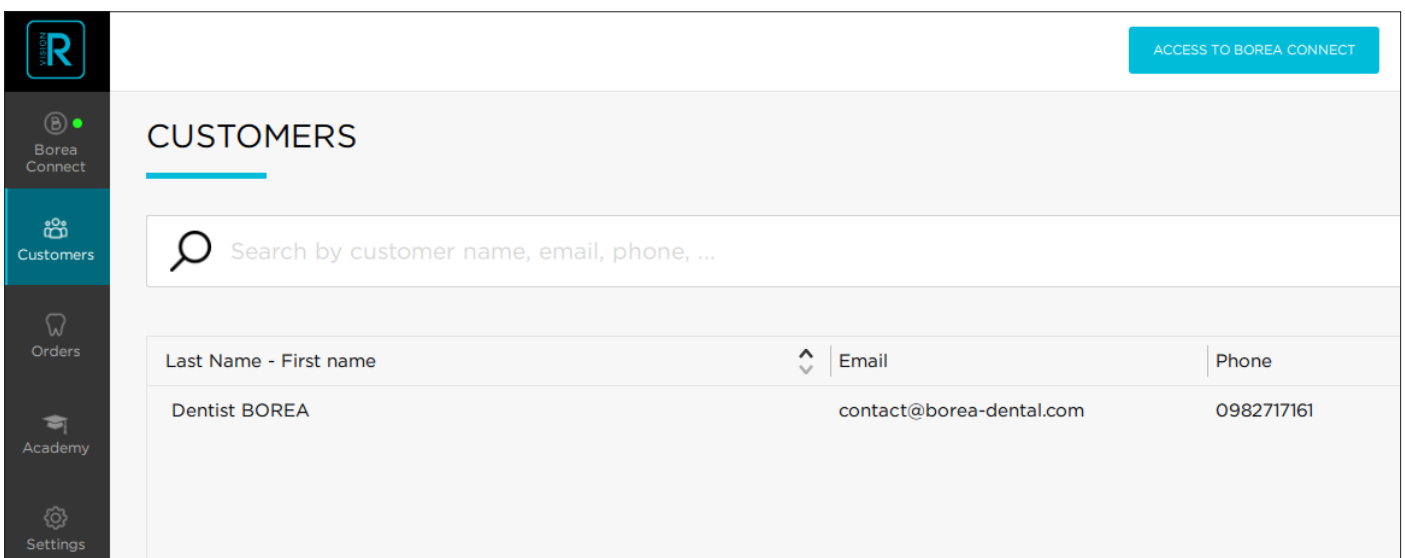

The screenshot shows the 'CUSTOMERS' section of the Raypicker Vision interface. At the top, there is a button for 'ACCESS TO BOREA CONNECT'. Below this is a search bar with the placeholder text 'Search by customer name, email, phone, ...'. The main part of the interface is a table with the following columns: Last Name - First name, Email, and Phone. The first row of the table is highlighted.

Last Name - First name	Email	Phone
Dentist BOREA	contact@borea-dental.com	0982717161

A click on the name of the dental practice allows you to view or sort the items and orders sent by the latter.

The screenshot shows the 'DENTIST BOREA' interface. At the top right, there are buttons for 'IMPORT (.rpk)', 'ADD PICTURE', 'ADD 3D', and 'ADD SHADE'. Below these, there are tabs for 'ELEMENTS' and 'ORDERS', with 'ORDERS' being the active tab. On the left, under 'Order sorting tools', there is a 'Date' dropdown menu and a 'Search' input field. Below this, there are radio buttons for 'Sort by date' with options 'Newest' (selected) and 'Oldest'. There are also radio buttons for 'Hide orders' with options 'more than 15 days', 'more than 1 month', 'more than 3 month', and 'more than 6 month'. The main table displays a list of orders with columns: 'No.', 'Date / Time', 'Patient name', and 'Elements'. The first row shows order number 638, dated 19/01/2022, for patient William Smith, with elements R, a cube icon, and a document icon.

7. ANNEX

7.1 Port configuration

If the computer is behind a firewall or a network device, such as a router, it may be necessary to modify the configuration to allow the Rayplicker device or the Rayplicker mobile application to communicate with the Rayplicker Vision software on the computer.

This operation is sometimes called “port opening”.

Rayplicker Vision software needs the following ports to be opened :

(Mandatory for using Rayplicker Vision software)

- Port 3306 (TCP)

Rayplicker mobile application «Rayplicker Pics App Solution»:

- Port 7777 (UDP et TCP)
- Port 7778 (UDP et TCP)

Note :

Communications between the different elements of the Rayplicker solution take place on the local network. All the different elements of the Rayplicker Vision solution need to be connected to the same local network.

If you encounter difficulties to configure your network, call your network administrator or your internet provider to open the ports above, used by the Rayplicker solution.

7.2 Regulatory



The Rayplicker Vision has the CE mark in accordance with regulation (EU) 2017/745 relating to class I medical devices.

Manufacturer: Borea SAS

Borea designs, develops and markets the Rayplicker Vision and the Borea connect.

Borea undertakes to carry out repair actions in accordance with the conditions of sale.

Here is the list of harmonized standards and common specifications applied to the Rayplicker Vision and the Borea Connect platform

ISO 13485

Medical devices - Quality management systems - Requirements for regulatory purposes.

ISO 14971

Medical devices — Application of risk management to medical devices

NF EN 62304

Medical device software - Software life-cycle processes

NF EN 62366-1

Medical devices - Part 1: Application of usability engineering to medical devices

7.3 General Data Protection Regulation

The BOREA company provides the User of the software with a means of collecting and transmitting data and is, as such, considered as a service provider and is therefore not responsible for the processing of personal data.

However, BOREA in its capacity as service provider, informs the User that it is required to take all necessary measures with national or international organizations for the protection and security of personal data (CNIL, etc.) in order to preserve the rights of the persons whose personal data may be collected and transmitted to another user.

The User of this software must ensure that the patient consents to the collection of his personal data. In accordance with the computer and freedom laws, the person whose personal information has been collected retains the right to access and modify this information.

It should be noted that this personal data is collected by the User for the sole purpose of benefiting from the information of a person's tooth shade with a view to prosthetic production. For the same purpose, this personal data may also be transmitted by a User to another User of his choice.

BOREA informs the User that the data collected is temporarily stored in a data exchange space (Cloud) for the time necessary for the prosthesis to be produced. The data exchanged is not sensitive data. These data are encrypted and access to this database is controlled. These data are automatically deleted from the data exchange space at the end of the prosthetic production. Only local copies are kept.

Using the cloud, data is encrypted and stored only temporarily.

The data includes:

- Information relating to the colorimetry of the patient's tooth.
- The patient's data, they are personal but not medical (name, age, photo).
- Data relating to prosthesis orders (dentist, prosthetist, product ordered, etc.)

7.4 Contact

BOREA SAS,

6 Allée Duke Ellington, 87100 Limoges Cedex, France.

+33 (0)9 83 71 71 61 - contact@borea-dental.com - www.borea-dental.com

