




DISINFECTION AND STERILIZATION PROCEDURES


STEPS	CALIBRATION TIPS	DEVICE RAYPLICKER COBRA
- 1 - DISINFECTION		
- 2 - RINSING		
- 3 - STERILIZATION	AUTOCLAVE STERILIZATION	

Disinfectant wipes for surfaces of non-invasive medical devices with bactericidal, fungicidal, virucidal and tuberculocidal properties. Please follow the manufacturer's instructions (contact time required).
This device disinfection protocol is mandatory after each use to avoid cross-contamination.

RISKY AREAS IN CASE OF EXCESSIVE USE OF DISINFECTANTS

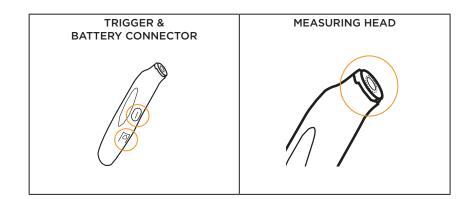

NON-COMPLIANT PRODUCTS AND PROCESSES

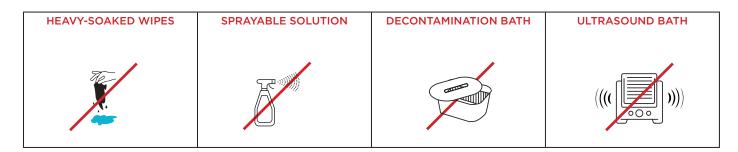

Disinfection and sterilization procedures for the Rayplicker Cobra (EN_09.2022)



